


Table of Contents

| | Page |
|--|-----------|
| Diagram: Instrument Classification | 2 |
| Instrument Classification Overview | 3 |
| Instrument Grouping | 6 |
| - Clinical Chemistry Instruments | 6 |
| - Immunochemistry Instruments | 14 |
| - Haematology Instruments | 17 |
| - Microbiology Instruments | 22 |
| - Other Clinical Instruments | 23 |
| - Data Management Systems | 23 |
| Alphabetical Order by Company | 24 |
| Alphabetical Order by Instrument Name | 36 |

Diagram Instrument Classification Level 1 - 2

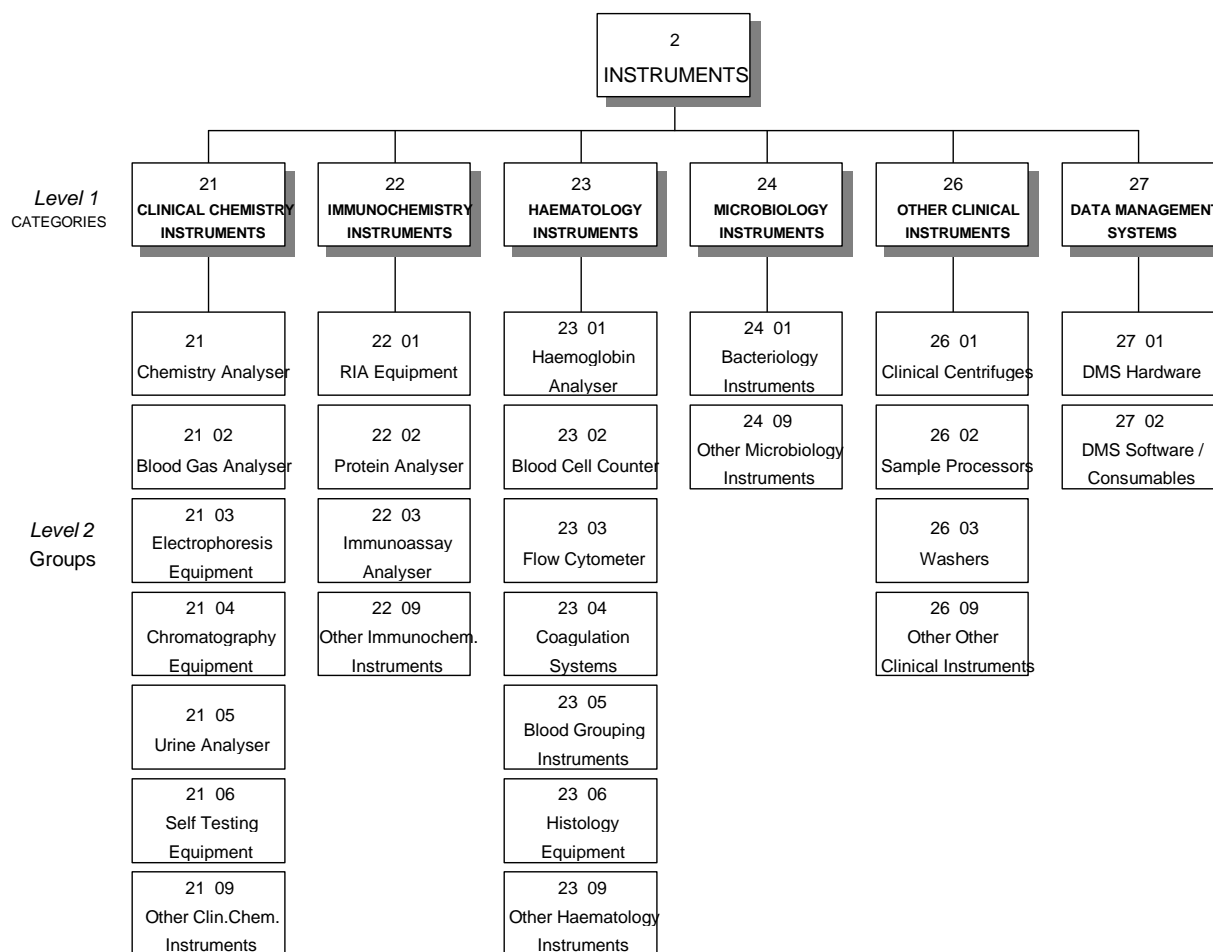

Level 3 Subgroups ==> see following pages

| EDMA CODE | Company | Instrument-Name | Page |
|-----------|---------|---|------|
| | | <u>Instrument Classification Overview</u> | |
| | | <u>Level 1 - 3</u> | |
| 2 | | INSTRUMENTS | |
| 21 | | CLINICAL CHEMISTRY INSTRUMENTS | 6 |
| 21 01 | | Chemistry Analyser | |
| 21 01 01 | | Manual Photometer and Spectrophotometer | |
| 21 01 11 | | Dedicated Glucose Systems | 7 |
| 21 01 12 | | Dedicated Glycated Haemoglobin /HbA1 Systems | |
| 21 01 19 | | Other Dedicated Single-Parameter CC Systems | |
| 21 01 29 | | Dedicated Multi-Parameter CC Systems | |
| 21 01 31 | | Small Manual and Semi-automated CC Systems | |
| 21 01 32 | | Semi-automated CC Analyser | |
| 21 01 41 | | Small Automated CC Analyser | 8 |
| 21 01 42 | | Medium Automated CC Analyser | 9 |
| 21 01 43 | | Large Automated CC Analyser | |
| 21 01 44 | | Extra large Automated CC Analyser | |
| 21 01 51 | | Electrolyte - Flame photometer | 10 |
| 21 01 52 | | Electrolyte/ISE only | |
| 21 01 53 | | Electrolyte/ISE and other parameter | |
| 21 02 | | Blood Gas Analyser | |
| 21 02 01 | | Blood Gas (pO2 / pCO2 + pH) | |
| 21 02 02 | | Blood Gas and Electrolytes | 11 |
| 21 02 03 | | Blood Gas and CO-Oximeter | |
| 21 02 04 | | Blood Gas, Electrolytes and CO-Oximeter | |
| 21 02 06 | | Blood Gas, Electrolytes, CO-Oximeter and Other Parameters | |
| 21 02 07 | | CO-Oximeter | |
| 21 02 09 | | Other Blood Gas Instruments | |
| 21 03 | | Electrophoresis Equipment | 12 |
| 21 03 01 | | Manual Electrophoresis | |
| 21 03 02 | | Densitometers | |
| 21 03 03 | | Automated integrated Electrophoresis Systems | |
| 21 04 | | Chromatography Equipment | |
| 21 05 | | Urine Analyser | 13 |
| 21 05 01 | | Manual Urine Analyzer | |
| 21 05 02 | | Small Automated Urine Analyzer | |
| 21 05 03 | | Medium Automated Urine Analyzer | |
| 21 05 04 | | Large Automated Urine Analyzer | |
| 21 06 | | Self Testing Equipment (Clin.Chem.) | |
| 21 06 01 | | Blood Glucose Meter | |
| 21 06 02 | | Cholesterol Meter | |
| 21 06 03 | | Lactate Meter | |
| 21 06 11 | | Multiparameter CC Meter | |
| 21 09 | | Other Clinical Chemistry Instruments | |

| EDMA CODE | Company | Instrument-Name | Page |
|-----------|---|-----------------|------|
| 22 | IMMUNOCHEMISTRY INSTRUMENTS | | 14 |
| 22 01 | RIA Equipment | | |
| 22 01 01 | RIA Counter | | |
| 22 02 | Protein Analyser | | |
| 22 02 01 | Small Protein Analyser | | |
| 22 02 02 | Large Protein Analyser | | |
| 22 03 | Immunoassay Analyser | | |
| 22 03 01 | Manual I.A. Instruments / Readers | | |
| 22 03 02 | Semi-automated I.A. Systems | | 15 |
| 22 03 03 | Automated I.A. Systems | | 16 |
| 22 03 04 | Batch / High throughput I.A. Systems | | |
| 22 03 05 | Nucleic Acid Processors | | |
| 22 09 | Other Immunochemistry Instruments | | |
| 23 | HAEMATOLOGY INSTRUMENTS | | 17 |
| 23 01 | Haemoglobin Analyser | | |
| 23 01 01 | Dedicated Total Haemoglobin Analyser | | |
| 23 02 | Blood Cell Counter | | |
| 23 02 01 | No differential Blood Cell Counter | | |
| 23 02 02 | 2 / 3 part differential Blood Cell Counter | | 18 |
| 23 02 03 | 5 part differential low / medium end Blood Cell Counter | | |
| 23 02 04 | 5 part differential high end Blood Cell Counter | | 19 |
| 23 02 11 | Dedicated Reticulocyte Analyser | | |
| 23 03 | Flow Cytometer | | |
| 23 03 01 | Flow Cytometer without Cell sorter | | |
| 23 03 02 | Flow Cytometer with Cell sorter | | |
| 23 04 | Coagulation Systems | | 20 |
| 23 04 01 | Manual Coagulation Instruments | | |
| 23 04 02 | Semi-automated Coagulation Systems | | |
| 23 04 03 | Fully-automated Coagulation Systems | | 21 |
| 23 04 04 | Aggregometer | | |
| 23 04 05 | Selftesting Equipment (Coagulation) | | |
| 23 05 | Blood Grouping Instruments | | |
| 23 05 01 | Blood Grouping Instruments | | |
| 23 06 | Histology Equipment (excl.microscopes) | | |
| 23 06 01 | General Histology Instruments | | |
| 23 06 02 | Microtomes | | |
| 23 09 | Other Haematology Instruments | | |
| 23 09 01 | Sediment rate Instruments | | |

| EDMA CODE | Company | Instrument-Name | Page |
|-----------|---------|---|------|
| 24 | | MICROBIOLOGY INSTRUMENTS | 22 |
| 24 01 | | Bacteriology Instruments | |
| 24 01 01 | | Plate pouring Instruments | |
| 24 01 02 | | Susceptibility and / or ID-systems | |
| 24 01 03 | | Blood Culture Systems | |
| 24 01 04 | | Dedicated Urine Screening MB Instruments | 23 |
| 24 09 | | Other Microbiology Instruments | |
| 26 | | OTHER CLINICAL INSTRUMENTS | |
| 26 01 | | Clinical Centrifuges | |
| 26 02 | | Sample Processors | |
| 26 02 01 | | Clinical Chemistry Sample Processors | |
| 26 02 02 | | Immuno Assays Sample Processors | |
| 26 02 03 | | Haematology Sample Processors | |
| 26 02 04 | | Microbiology Sample Processors | |
| 26 02 09 | | Multiple Purpose Sample Processors | |
| 26 03 | | Washers | |
| 26 03 02 | | Immuno Assays Washers | |
| 26 03 03 | | Haematology Washers | |
| 26 03 09 | | Other Washers | |
| 26 09 | | Other Other Clinical Instruments | |
| 27 | | DATA MANAGEMENT SYSTEMS | |
| 27 01 | | Data Management Hardware | |
| 27 02 | | Data Management Software/Consumables | |

| EDMA CODE | Company | Instrument-Name |
|-----------------------------------|---|--|
| <u>Instrument Grouping</u> | | |
| 2 | INSTRUMENTS | |
| 21 | CLINICAL CHEMISTRY INSTRUMENTS | |
| 21 01 | Chemistry Analyser | |
| 21 01 01 | Manual Photometer and Spectrophotometer | |
| | Bayer | ML 1 ML2 ML3 |
| | Beckman | Model 42 DU 5 |
| | BioMérieux | UV-VIS Jr UV-VIS 1 UV-VIS 2 VISUAL |
| | BioSystems | BTS 302 BTS 305 BTS 310 |
| | Boehringer Mannheim | Photometer 4010 Photometer 4020 Photometer 5010 |
| | Eppendorf | PCP 6121 ECOM 6122 ECOM 6124 F |
| | Gilford | 103 203 |
| | Hycel | ISIS |
| | Lange (Dr. Lange) | LP 1 LP 3 LP 6A LP 400 LP 500 Miniphotometer 8 Miniphotometer 20 |
| | Merck | Eclipse Eclipse Plus |
| | Milton-Roy | Spectronic 1001+ Spectronic 1101 Spectronic 1201 Spectronic 20 / 20 D Spectronic 21 DV Spectronic 21 MV Spectronic 21 UVD Spectronic 3000 Spectronic 301 Spectronic 401 Spectronic 501 Spectronic 601 |
| | Perkin-Elmer | Lambda 11 Lambda 12 Lambda 14 |
| | Riele | PMC 2000 PM 210 PM 310 |
| | Unicam | PU 8610 PU 8620 |
| | Vitatron | IFP ISP |

| EDMA CODE | Company | Instrument-Name |
|-----------|---|--------------------------|
| 21 01 11 | Dedicated Glucose Systems | |
| | Beckman | Glucose-Analyzer 2 |
| | Eppendorf | EBIO Compact |
| | Radiometer | ABL System 625 |
| | Yellow Springs | YSI |
| 21 01 12 | Dedicated Glycated Haemoglobin /HbA1 Systems | |
| | ARKRAY KDK | Hi-Auto A1c HA 8140 |
| | Bayer | DCA 2000 |
| | Bio-Rad | DIAMAT |
| | | DiaSTAT |
| | | VARIANT |
| | Chiron | Glycomat |
| | Kontron | NN |
| | Menarini | HA 8110 |
| | | HA 8121 |
| | | HA 8140 |
| | Merck | Hitachi L 9000 |
| 21 01 19 | Other Dedicated Single-Parameter CC Systems | |
| | Analox Instruments | LM10 |
| | Beckman | Creatinine-Analyzer 2 |
| | | Urea-Analyzer 2 |
| | Elvilogos | Bilirubinometer |
| 21 01 29 | Dedicated Multi-Parameter CC Systems | |
| | Analox Instruments | P-GM7 micro-Stat |
| | Eppendorf | EBIO Plus |
| 21 01 31 | Small Manual and Semi-automated CC Systems | |
| | Abbott | Vision |
| | Bayer | Seralyzer |
| | Boehringer Mannheim | Reflotron |
| | | Reflotron Sprint |
| | Cholestech | L.D.X |
| | Ortho Diag. Systems (J&J) | Vitros DT 60/Vitros DT60 |
| | Eppendorf | SPOTCHEM |
| | Menarini | SPOTCHEM |
| | Merck | EASY ST |
| | Roche | COBAS Ready (=SPOTCHEM) |
| 21 01 32 | Semi-automated CC Analyser | |
| | Beckman | Clinical System 700 |
| | BPC BioSED | NN |
| | Eppendorf | EPAC 6140 |

| EDMA CODE | Company | Instrument-Name |
|-----------|------------------------------------|---|
| 21 01 41 | Small Automated CC Analyser | |
| | Abbott | ABA 100 / 200 VP Spectrum |
| | Bayer | RA 50 RA 500 RA 1000 RA XT |
| | Beckman | AS 4 / AS 8 Synchron CX3 |
| | Boehringer Mannheim | Autolab Hitachi 704 Hitachi 705 Hitachi 902 Hitachi 904 |
| | Chimica Diagnostica | Naxos |
| | Chiron | EXPRESS |
| | Dade (Dupont) | Dimension 380 Dimension ES |
| | Diagnostic Testing | Piccolo |
| | Eppendorf | ACP 5040 EASY EPOS ELAN |
| | Hycel | LISA 200 LISA 300 |
| | Instrumentation Laboratory | Monarch 1000 |
| | Kone | Progress Progress Plus Specific Specific Supra Pro |
| | Menarini | Classic/Artax |
| | Merck | Selectra |
| | Olympus | AU 200 |
| | Roche | COBAS BIO COBAS MIRA COBAS MIRA S COBAS MIRA PLUS COBAS FARA COBAS FARA II |
| | Schiaparelli | ACE |
| | Sigma | SD2000 |
| | Wako | 20R |

| EDMA CODE | Company | Instrument-Name | |
|----------------------------|-------------------------------------|---|----------------------------|
| 21 01 42 | Medium Automated CC Analyser | | |
| | Abbott | EPx | |
| | Bayer | RA2000 OPERA | |
| | Beckman | Synchron CX 3 DELTA Synchron CX 4 Synchron CX 4 DELTA Synchron CX 5 Synchron CX 5 DELTA | |
| | Boehringer Mannheim | Hitachi 911 | |
| | Coulter | Optichem 500 | |
| | Eppendorf | ERIS ETEC | |
| | Instrumentation Laboratory | Monarch PLUS Monarch 2000 | |
| | Kone | Delta Dynamic Optima Ultra | |
| | Hycel | LISA 400 | |
| | Menarini | Falcor 300 Falcor 600 | |
| | Nova | Nucleus | |
| | Olympus | AU 510 AU 560 | |
| | Ortho Diag. Systems (J&J) | Vitros 250 Vitros 500 | |
| | Wako | 30R | |
| | 21 01 43 | Large Automated CC Analyser | |
| | | American Monitor | Perspective/Excel |
| | | Bayer | AXON DAX 24 DAX 48 |
| | | Beckman | Synchron CX 7 / CX7 Delta |
| | | Boehringer Mannheim | Hitachi 717 Hitachi 917 |
| Dade (Dupont) | | Paramax-RX Dimension 760 Dimension AR Dimension XL | |
| Instrumentation Laboratory | | ILab 900 | |
| Merck | | MEGA | |
| Olympus | | AU 600 | |
| Ortho Diag. Systems (J&J) | | Vitros 750 XRC Vitros 950 IRC/Vitros 950 | |
| Roche | | COBAS INTEGRA | |
| 21 01 44 | | Extra large Automated CC Analyser | |
| | | Bayer | CHEM 1 DAX 72 DAX 96 |
| | | Boehringer Mannheim | HIT 737 HIT 747 Series |
| | Instrumentation Laboratory | ILab 1800 | |
| | Olympus | AU 800 AU 1000 AU 5000 Series AU 5200 Series | |

| EDMA CODE | Company | Instrument-Name | |
|-----------|--|---------------------------|----------------|
| 21 01 51 | Electrolyte - Flame photometer | | |
| | Hycel | PHF 104 PHF 106 | |
| | Instrumentation Laboratory | IL 943 | |
| 21 01 52 | Electrolyte/ISE only | | |
| | AVL | 9180 Electrolyte Analyser | |
| | Beckman | E2A | |
| | Hycel | EASYLYTE | |
| | Instrumentation Laboratory | IL 614, 644, 654 | |
| YSI | EasyLyte | | |
| 21 01 53 | Electrolyte/ISE and other parameter | | |
| | Beckman | ELISE | |
| 21 02 | Blood Gas Analyser | | |
| 21 02 01 | Blood Gas (pO₂ / pCO₂ + pH) | | |
| | AVL | AVL 945 | |
| | | AVL 990 | |
| | | AVL 995 | |
| | | OPTI 1 | |
| | | Compact 1 | |
| | | Compact 2 | |
| | Chiron | CCD 238 | |
| | | CCD 248 | |
| | | CCD 278 | |
| | | CCD 280 | |
| | | CCD 840 | |
| | | Hewlett Packard | i-STAT |
| | Instrumentation Laboratory | IL 1304 | |
| | | IL 1306 | |
| | | IL 1312 | |
| | | IL 1420 | |
| | | IL 1610 | |
| | | IL 1620 | |
| | | IL BG3 | |
| | | Nova | Stat Profile 3 |
| | | Radiometer | ABL 5 |
| | ABL 30 | | |
| | ABL 300 | | |
| | ABL 330 | | |
| | ABL 500 | | |
| | ABL 510 | | |
| ABL 520 | | | |

| EDMA CODE | Company | Instrument-Name | |
|--------------------------|------------------------------------|---|--------------------|
| 21 02 02 | Blood Gas and Electrolytes | | |
| | Chiron | CCD 348 CCD 850 CCD 860 | |
| | Diametrics | IRMA | |
| | Instrumentation Laboratory | IL 1400 IL 1405 IL 1430 IL 1630 IL 1640 IL 1650 GEM Premier GEM STAT GEM 6+ GEM Premier Plus | |
| | Nova Biomedical | Stat Profile1,2,4,5,7 Stat Profile Plus 9,10 Stat Profile Ultra | |
| | Radiometer | ABL 4 ABL 505 ABL 620 | |
| | AVL | OMNI | |
| | 21 02 03 | Blood Gas and CO-Oximeter | |
| | 21 02 04 | Blood Gas, Electrolytes and CO-Oximeter | |
| | | AVL | OMNI |
| | | Chiron | CCD 845 CCD 855 |
| | | Instrumentation Laboratory | Synthesis 25 / 35 |
| | Radiometer | ABL 620 | |
| | 21 02 06 | Blood Gas, Electrolytes, CO-Oximeter and Other Parameters | |
| Chiron | | CCD 865 | |
| | Nova | Stat Profile Ultra | |
| 21 02 07 | CO-Oximeter | | |
| | AVL | AVL 912 | |
| | Chiron | CCD 270 CCD 815 | |
| | Instrumentation Laboratory | IL 482 IL 682 | |
| | Radiometer | OSM 3 | |
| 21 02 08 | Osmometer | | |
| Gonotec | Osomat 030/030D Osomat 050 | | |
| Slamed | Osmometer 800 cl | | |
| Roebing | Micro-Osmometer | | |
| Vitech Scientific | Model 3900 | | |
| Wescor | Vapro | | |
| 21 02 09 | Sweat Analyzer | | |
| Wescor | Sweat-Chek Analyzer | | |
| 21 02 90 | Other Blood Gas Instruments | | |

| EDMA CODE | Company | Instrument-Name |
|-----------|---|---|
| 21 03 | Electrophoresis Equipment | |
| 21 03 01 | Manual Electrophoresis | |
| | Beckman | PARAGON |
| | Cosmo | FED 3200 |
| | Helena | NN |
| | Sebia | NN |
| 21 03 02 | Densitometers | |
| | Beckman | APPRAISE |
| | Helena | NN |
| | Olympus | Fractoscan Fractoscan Junior |
| | Sebia | HYDRASYS |
| 21 03 03 | Automated integrated Electrophoresis Systems | |
| | Beckman | APPRAISE PARAGON CZE 2000 |
| | Eppendorf (JOOKOO) | CTE 1000 CTE 5000 |
| | Helena | Concept 2000 REP Cardio REP PRINCE-CE AUTOIFE |
| | Menarini | HS 7 |
| | Olympus | HITE SYSTEM 310 HITE SYSTEM 320 HITE SYSTEM 620 |
| | Sebia | HYDRASYS |
| 21 04 | Chromatography Equipment | |

| EDMA CODE | Company | Instrument-Name |
|-----------|---|---|
| 21 05 | Urine Analyser | |
| 21 05 01 | Manual Urine Analyser | |
| | Menarini | MiniAution |
| 21 05 02 | Small Automated Urine Analyser | |
| | Bayer | Clinitek 50 Clinitek 100 |
| | Boehringer Mannheim | Urilux Minitron |
| | IMACO | URIMAC |
| 21 05 03 | Medium Automated Urine Analyser | |
| | Bayer | Clinitek 200 Clinitek 200 + |
| | Boehringer Mannheim | Miditron Miditron Junior Urotron RL 9 |
| | Behring | RAPIMAT |
| 21 05 04 | Large Automated Urine Analyser | |
| | Bayer | Clinitek Atlas |
| | Boehringer Mannheim | Supertron |
| | IRIS | 900UDx |
| | Menarini | SuperAution |
| | Sysmex | UF-100 |
| | Wako | NN |
| | Yeong Deong | NN |
| 21 06 | Self Testing Equipment (Clin.Chem.) | |
| 21 06 01 | Blood Glucose Meter | |
| 21 06 02 | Cholesterol Meter | |
| 21 06 03 | Lactate Meter | |
| 21 06 11 | Multi-Parameter CC Meter | |
| 21 09 | Other Clinical Chemistry Instruments | |

| EDMA CODE | Company | Instrument-Name |
|-----------|--|-----------------------------|
| 22 | IMMUNOCHEMISTRY INSTRUMENTS | |
| 22 01 | RIA Equipment | |
| 22 01 01 | RIA Counter | |
| 22 02 | Protein Analyser | |
| 22 02 01 | Small Protein Analyser | |
| | Beckman | ICS |
| | Behring | TurbiTimer |
| | Bio-Whittaker | Fiax |
| | Nycomed | Card Reader |
| | Orion Diagnostica | Turbox |
| | | QuikRead 3 |
| 22 02 02 | Large Protein Analyser | |
| | Bayer | DPA-1 |
| | Behring | BN 100 |
| | | BNA |
| | | BN II |
| | Beckman | Array 2.0 |
| | | Array 360 |
| | | IMMAGE |
| | Boehringer Mannheim | KeySys |
| | Sanofi Diagnostics Pasteur | QM 300 |
| 22 03 | Immunoassay Analyser | |
| 22 03 01 | Manual I.A. Instruments / Readers | |
| | Abbott | Matrix |
| | | Quantum |
| | | Quantum II |
| | Behring | Elisa-Photometer |
| | | Elisa-Reader 301 |
| | | Elisa-Reader 311 |
| | | Berilux 250 |
| | | Microtrack Reader SE System |
| | | ECOM 6123 D |
| | Biochem Immunosystems | Serazyme I |
| | | Serazyme II |
| | BioMerieux | Axia Microreader |
| | | Axia 2 Reader |
| | Boehringer Mannheim | ES 11 |
| | | ES 22 |
| | | ES 33 |
| | Chiron | Magic Lite I |
| | Dynatech | System 5000 |
| | Eppendorf | ECOM 6123 D |
| | Hybritech | Photon II |
| | Merck | Eclair |
| | | LM-8 |
| | Murex | Micro ELISA Reader 7000 |
| | | Micro ELISA MRX Reader |
| | Organon Teknika | Microelisa Reader 100 |
| | | Microelisa System |
| | Ortho Diagnostic Systems | Auto Reader 3 |
| | Sanofi Diagnostics Pasteur | LP 400 |

| EDMA CODE | Company | Instrument-Name |
|-----------|------------------------------------|---|
| 22 03 02 | Semi-automated I.A. Systems | |
| | Abbott | ADx IMx / IMx Select TDx / TDxFLx |
| | Behring | BeriLux 400 BEP II OPUS OPUS PLUS ETS Plus Solaris |
| | Biochem Immunosystems | SR 1 |
| | BioMerieux | VIDAS Mini-VIDAS |
| | Boehringer Mannheim | ES 300 ElecSys 1010 |
| | Byk-Sangtek | LIA-mat S 300 |
| | Chiron | Magic Lite II Magic Lite II+ Magic Lite SQ Allergy System |
| | Dade | Stratus I Stratus II |
| | DPC | Milenia Max Immulite |
| | Dade (Dupont) | ACA III ACA V ACA SX ACA STAR |
| | Hybritech | Photon Era |
| | Ortho Diag. Systems (J&J) | Amerlite |
| | Pharmacia | UniCAP |
| | Radim | BRIO |
| | Roche | COBAS EIA System |
| | Sorin | ETI-SYSTEM |
| | Tosoh | AIA 600 |
| | Wallac / Pharmacia | Delfia |

| EDMA CODE | Company | Instrument-Name | |
|----------------------------|--|---|--------------------------|
| 22 03 03 | Automated I.A. Systems | | |
| | Abbott | AxSYM | |
| | Bayer | Immuno-I | |
| | Behring | OPUS Magnum | |
| | Biochem Immunosystems | Labotec | |
| | Boehringer Mannheim | ES 600 | |
| | | ES 700 | |
| | | ElecSys 2010 | |
| | Chiron | ACS 180 | |
| | | ACS 180 PLUS | |
| | | Centaur | |
| | CIS-Bio | Cispack 4200 | |
| | DPC | Immulite 2000 | |
| | Hycor | HY-TEC 288 | |
| | Kone | Quartus | |
| | Lisabio | Ligand Immuno System Assay | |
| | Merck (Biotrol) | MAGIA 7000 | |
| | | MAGIA 8000 | |
| | Nichols Institute Diagnostic | Advantage | |
| | Organon Teknika | Tektime | |
| | Ortho Diag. Systems (J&J) | Amerlite PC | |
| | | Vitros ECI | |
| | Radim | Ario | |
| | Roche | COBAS CORE | |
| | | COBAS CORE II | |
| | Rosys | Plato 1300 | |
| | Sanofi Diagnostics Pasteur | Access | |
| | Sorin | ETI-LAB | |
| | Tosoh | AIA 1200 | |
| | Wallac / Pharmacia | AutoDELFIA | |
| | | Unicap 100 | |
| | 22 03 04 | Batch / High throughput I.A. Systems | |
| | | Abbott | Commander / FPC PRISM |
| Beckman | | Image | |
| Behring | | BEP III | |
| | | BEP XL (Micro Trak XL) | |
| Bio-Rad | | Radius | |
| BIO-TEK | | ELx808 | |
| DPC / Biermann | | MAX | |
| Dynatech | | System 7000 | |
| Hamilton | | Microlab F.A.M.E. | |
| Hycor | | HY TEC EIA System | |
| Merck | | MIOS | |
| Murex | | DIAS System | |
| | | MIAS System | |
| Organon Teknika | | MPP 3000 | |
| Ortho Diagnostic Systems | | Summit | |
| Rosys | | Plato 3300 | |
| Sanofi Diagnostics Pasteur | | AMS/LP 400 | |
| | | Sonata | |
| Sorin | | Omni System | |
| 22 03 05 | | Nucleic Acid Processors | |
| | | Abbott | LCx |
| | | Becton Dickinson | ProbeTec |
| | Organon Teknika | NASBA QR System | |
| | Perkin Elmer | GenAmp PCR system 2400 | |
| Roche | COBAS Amplicor | | |
| 22 09 | Other Immunochemistry Instruments | | |

| EDMA CODE | Company | Instrument-Name |
|-----------|---|--|
| 23 | HAEMATOLOGY INSTRUMENTS | |
| 23 01 | Haemoglobin Analyser | |
| 23 01 01 | Dedicated Total Haemoglobin Analyser | |
| 23 02 | Blood Cell Counter | |
| 23 02 01 | No differential Blood Cell Counter | |
| | Abbott | CELL-DYN 300 CELL-DYN 400 CELL-DYN 500 CELL-DYN 610 CELL-DYN 700 CELL-DYN 800 CELL-DYN 900 |
| | Becton-Dickinson | QBC I QBC II QBC Autoread |
| | Biochemical Systems | Hema-Check 5 |
| | Biochem Immunosystems | 130 150 170 7500 8000 |
| | Coulter | CBC-5 M430 MD 8 ZM M530 |
| | Kone | AC 900 AC 920 |
| | Nihon Kohden | Celltak MEK-5100 |
| | Sysmex | F-520 F-820 |

| EDMA CODE | Company | Instrument-Name | |
|-----------|---|---|--|
| 23 02 02 | 2 / 3 part differential Blood Cell Counter | | |
| | Abbott | CELL-DYN 1300 CELL-DYN 1400 CELL-DYN 1600 CELL-DYN 1700 | |
| | Bayer | H1JR | |
| | Coulter | T540 T660 MD 16 MD II S770 | |
| | Diatron | Twincell | |
| | Hycel | CELLY HEMACELL | |
| | Kone | AC 970 | |
| | Nihon Kohden | Celltak Mini Celltak-Auto | |
| | Roche | COBAS MICROS COBAS MINOS ST COBAS MINOS STE COBAS MINOS STX COBAS MINOS STEX COBAS MINOS VET | |
| | Biochem Immunosystems | 9000 9100 + 9118 + 9120 + | |
| | SEAC | GENIUS | |
| | Sysmex | K-800 K-1000 | |
| | 23 02 03 | 5 part differential low / medium end Blood Cell Counter | |
| | | Abbott | CELL-DYN 2000 |
| | | Bayer | H1 |
| | | Biochemical Systems | Hema-Check 13 |
| | | Coulter | JS JR T890 S880 Onyx |
| | | Hycel | HEMACELL PLUS |
| | | Roche | COBAS HELIOS LMG COBAS HELIOS 5 Diff. |
| | | Sysmex | NE-1500 K-4500 |

| EDMA CODE | Company | Instrument-Name | |
|------------------|--|--|--------|
| 23 02 04 | 5 part differential high end Blood Cell Counter | | |
| | Abbott | CELL-DYN 3000 CELL-DYN 3500 CELL-DYN 4000 | |
| | Bayer | H 1 E H 2 H 3 RTC H 3 RTX | |
| | Coulter | STKR STKS MAXM ST | |
| | Lisabio | Gen S | |
| | Roche | Hemacell/Hemacell Plus COBAS ARGOS LMG COBAS ARGOS 5 Diff. COBAS VEGA | |
| | Swelab | AC920 | |
| | Sysmex | SF-3000 SE-9000 NE-8000 | |
| | 23 02 11 | Dedicated Reticulocyte Analyser | |
| | | Sysmex | R-3000 |
| | | Sediment rate analyser | |
| | | COFIM | SR 50 |
| | Eurotec Medical System | VT-50/VT-75/VT-100 | |
| | ALIFAX | Test 1 | |
| 23 03 | Flow Cytometer | | |
| 23 03 01 | Flow Cytometer without Cell sorter | | |
| | Becton-Dickinson | FACScan FACStrak FACSCalibur FACSCount | |
| | Bio-Rad | NN | |
| | Coulter | Epics Profile II | |
| | Ortho Diag. Systems (J&J) | Cytonon Absolute | |
| | Partec | CA-II | |
| | Sysmex | R-2000/3000 | |
| | 23 03 02 | Flow Cytometer with Cell sorter | |
| Becton-Dickinson | | FACStarPlus FACSVantage FACSort | |
| Coulter | | Epics Elite | |
| Partec | PAS-II | | |

| EDMA CODE | Company | Instrument-Name |
|-----------|---|--|
| 23 04 | Coagulation Systems | |
| 23 04 01 | Manual Coagulation Instruments | |
| | Amelung | KC 4 KC 10 KC 10A |
| | Behnk | CL4 CL8 |
| | Behring | Fibrintimer II Fibrintimer 10 Chromotimer |
| | BioMerieux | Option 2-8 |
| | Boehringer Mannheim | Coaguheck/Coaguheck Plus |
| | ERMA | SSC-100 |
| | Helena | Cascade M-4 |
| | Labor | COA Data 1000-3000 COA System COA Screener |
| | Labsystems | FP 900 FP 910 |
| | LRE | Coatron F Coatron F II |
| | Nycomed | Thrombotrack |
| | Organon Teknika | Coag-a-Mate XM |
| | Ortho Diagnostic Systems (MLA) | Electra 700 Koagulab CTS |
| | Roche | Fibrometer |
| | Stago | STA 2 STA 4 STA 8 STA 888 |
| | Teco Medical Instruments | Coachrome IV |
| 23 04 02 | Semi-automated Coagulation Systems | |
| | Biodata | MCA 110 |
| | Behnk | Thrombolyzer Chrom |
| | Boehringer Mannheim / Stago | Coasys 110 |
| | Helena | Cascade 480 |
| | Instrumentation Laboratory | ACL 100 ACL 200 ACL 300 |
| | ITC-International Technidyne | ProTime Microcoagulation System |
| | LRE | Coatron Jr. Coatron Fx |
| | Organon Teknika | Coag-A-Mate X2 Coag-A-Mate RA 4 |
| | Ortho Diagnostic Systems (MLA) | Electra 800 Electra 900 Electra 900 C Koagulab 16-605 |

| EDMA CODE | Company | Instrument-Name |
|-----------|---|---|
| 23 04 03 | Fully-automated Coagulation Systems | |
| | Amelung | KC 40 |
| | Behnk | Thrombolyser Thromboyzer Combi |
| | Behring | BFA BCT BCS |
| | BioMerieux | Hemolab |
| | Boehringer Mannheim / Stago | STA STA Compact |
| | Chiron | Biotrack 512 |
| | Instrumentation Laboratory | ACL 1000 ACL 2000 ACL 3000 ACL 3000p ACL 6000 ACL Futura |
| | Organon Teknika | Coag-A-Mate MDA Coag-A-Mate MTX |
| | Ortho Diagnostic Systems (MLA) | Electra 1000 C Electra 1400 C Electra 1600 C |
| | Stratec | Stracomat |
| | Sysmex / Dade | CA-1000 CA-5000 CA-6000 |
| 23 04 04 | Aggregometer | |
| | Biodata | PAP 4 |
| | Ortho Diag. Systems / Dade | PFA-100 |
| 23 04 05 | Selftesting Equipment (Coagulation) | |
| 23 05 | Blood Grouping Instruments | |
| 23 05 01 | Blood Grouping Instruments | |
| | Lifescreeen | QUASAR 240 QUASAR 400 |
| | Menarini | BOSS |
| | Olympus | PK 80 PK 7100 PK 7200 |
| | Ortho Diag. Systems (J&J) | AutoVue |
| 23 06 | Histology Equipment (excl.microscopes) | |
| 23 06 01 | General Histology Instruments | |
| | Pap Smear Screening NEOPATH | AutoPap 300 QC System |
| 23 06 02 | Microtomes | |
| 23 09 | Other Haematology Instruments | |
| 23 09 01 | Sediment rate Instruments | |

| EDMA CODE | Company | Instrument-Name |
|-----------|---|--|
| 24 | MICROBIOLOGY INSTRUMENTS | |
| 24 01 | Bacteriology Instruments | |
| 24 01 01 | Plate pouring Instruments | |
| 24 01 02 | Susceptibility and / or ID-systems | |
| | Dade | Touchscan Autoscan 4 Microscan Walkaway 40 Microscan Walkaway 96 |
| | Becton Dickinson | Sceptor Autosceptor Sceptorpette |
| | BioMerieux | Vitek Junior Vitek 32 Vitek 60 Vitek 120 Vitek 240 mini API Uniscept Aladin ATB Expression |
| | Biokit | Videobact |
| | Difco | Pasco |
| | I2R | STRSCAN |
| | Mast | Radius Mastscan |
| | Radiometer | Sensititre |
| 24 01 03 | Blood Culture Systems | |
| | Becton Dickinson | Bactec 460 Tb Bactec 660 Bactec 730 Bactec 860 Bactec 9000 MB Bactec 9050 Bactec 9120 Bactec 9240 |
| | BioMerieux | Vital 200 Vital 1200 |
| | Difco | Sentinel ESP |
| | Organon Teknika | BacT/Alert 120 BacT/Alert 240 |
| | Sanofi Diagnostics Pasteur | Bio Argos |

| EDMA CODE | Company | Instrument-Name |
|-----------|---|--------------------------------------|
| 24 01 04 | Dedicated Urine Screening MB Instruments | |
| | BioMerieux | Bact-T-Screen 2000 URIMAT |
| | Coral Biotechnology | Coral Wave 120 |
| | Difco | Questor |
| | Lumac | Biocounter M2300 Biocounter M3000 |
| | Orbec | Ramus |
| | Sysmex | UF-100 |
| 24 09 | Other Microbiology Instruments | |
| 26 | OTHER CLINICAL INSTRUMENTS | |
| 26 01 | Clinical Centrifuges | |
| 26 02 | Sample Processors | |
| 26 02 01 | Clinical Chemistry Sample Processors | |
| 26 02 02 | Immuno Assays Sample Processors | |
| | Abbott | PPC |
| | Beckman | BIOMEK 2000 |
| | Ortho Diag. Systems (J&J) | Summit Plus 2 Summit Processor |
| | Sanofi Diagnostics Pasteur | AMSS |
| | Tecan | GENESIS RSP 200 |
| 26 02 03 | Haematology Sample Processors | |
| 26 02 04 | Microbiology Sample Processors | |
| 26 02 09 | Multiple Purpose Sample Processors | |
| | Boehringer Mannheim | VS 250 PPV 1200 |
| 26 03 | Washers | |
| 26 03 02 | Immuno Assays Washers | |
| 26 03 03 | Haematology Washers | |
| 26 03 09 | Other Washers | |
| 26 09 | Other Other Clinical Instruments | |
| 27 | DATA MANAGEMENT SYSTEMS | |
| 27 01 | Data Management Hardware | |
| 27 02 | Data Management Software/Consumables | |

EDMA CODE

Company

Instrument-Name

Alphabetical Order by Company

| | | | | |
|----|----|----|------------------|-------------------|
| 21 | 01 | 31 | Abbott | Vision |
| 21 | 01 | 41 | Abbott | ABA 100 / 200 |
| 21 | 01 | 41 | Abbott | VP |
| 21 | 01 | 41 | Abbott | Spectrum |
| 21 | 01 | 42 | Abbott | EPx |
| 22 | 03 | 01 | Abbott | Matrix |
| 22 | 03 | 01 | Abbott | Quantum |
| 22 | 03 | 01 | Abbott | Quantum II |
| 22 | 03 | 02 | Abbott | ADx |
| 22 | 03 | 02 | Abbott | IMx / IMx Select |
| 22 | 03 | 02 | Abbott | TDx / TDxFLx |
| 22 | 03 | 03 | Abbott | AxSYM |
| 22 | 03 | 04 | Abbott | Commander / FPC |
| 22 | 03 | 04 | Abbott | PRISM |
| 22 | 03 | 05 | Abbott | LCx |
| 23 | 02 | 01 | Abbott | CELL-DYN 300 |
| 23 | 02 | 01 | Abbott | CELL-DYN 400 |
| 23 | 02 | 01 | Abbott | CELL-DYN 500 |
| 23 | 02 | 01 | Abbott | CELL-DYN 610 |
| 23 | 02 | 01 | Abbott | CELL-DYN 700 |
| 23 | 02 | 01 | Abbott | CELL-DYN 800 |
| 23 | 02 | 01 | Abbott | CELL-DYN 900 |
| 23 | 02 | 02 | Abbott | CELL-DYN 1300 |
| 23 | 02 | 02 | Abbott | CELL-DYN 1400 |
| 23 | 02 | 02 | Abbott | CELL-DYN 1600 |
| 23 | 02 | 02 | Abbott | CELL-DYN 1700 |
| 23 | 02 | 03 | Abbott | CELL-DYN 2000 |
| 23 | 02 | 04 | Abbott | CELL-DYN 3000 |
| 23 | 02 | 04 | Abbott | CELL-DYN 3500 |
| 23 | 02 | 04 | Abbott | CELL-DYN 4000 |
| 26 | 02 | 02 | Abbott | PPC |
| 23 | 04 | 01 | Amelung | KC 4 |
| 23 | 04 | 01 | Amelung | KC 10 |
| 23 | 04 | 01 | Amelung | KC 10A |
| 23 | 04 | 03 | Amelung | KC 40 |
| 21 | 01 | 43 | American Monitor | Perspective/Excel |
| 21 | 02 | 01 | AVL | AVL 945 |
| 21 | 02 | 01 | AVL | AVL 990 |
| 21 | 02 | 01 | AVL | AVL 995 |
| 21 | 02 | 01 | AVL | OPTI 1 |
| 21 | 02 | 01 | AVL | Compact 1 |
| 21 | 02 | 01 | AVL | Compact 2 |
| 21 | 02 | 04 | AVL | OMNI |
| 21 | 02 | 07 | AVL | AVL 912 |
| 21 | 01 | 01 | Bayer | ML 1 |
| 21 | 01 | 01 | Bayer | ML2 |
| 21 | 01 | 01 | Bayer | ML3 |
| 21 | 01 | 12 | Bayer | DCA 2000 |
| 21 | 01 | 31 | Bayer | Seralyzer |
| 21 | 01 | 42 | Bayer | RA2000 |
| 21 | 01 | 42 | Bayer | OPERA |
| 21 | 01 | 43 | Bayer | AXON |

| EDMA CODE | Company | Instrument-Name |
|-----------|------------------|-----------------------|
| 21 01 43 | Bayer | DAX 24 |
| 21 01 43 | Bayer | DAX 48 |
| 21 01 44 | Bayer | CHEM 1 |
| 21 01 44 | Bayer | DAX 72 |
| 21 01 44 | Bayer | DAX 96 |
| 21 05 02 | Bayer | Clinitek 50 |
| 21 05 02 | Bayer | Clinitek 100 |
| 21 05 03 | Bayer | Clinitek 200 |
| 21 05 03 | Bayer | Clinitek 200 + |
| 21 05 04 | Bayer | Clinitek Atlas |
| 22 02 02 | Bayer | DPA-1 |
| 22 03 03 | Bayer | Immuno-I |
| 23 02 02 | Bayer | H1JR |
| 23 02 03 | Bayer | H1 |
| 23 02 04 | Bayer | H 1 E |
| 23 02 04 | Bayer | H 2 |
| 23 02 04 | Bayer | H 3 RTC |
| 23 02 04 | Bayer | H 3 RTX |
| 21 01 41 | Bayer | RA 50 |
| 21 01 41 | Bayer | RA 500 |
| 21 01 41 | Bayer | RA 1000 |
| 21 01 41 | Bayer | RA XT |
| 21 01 01 | Beckman | Model 42 |
| 21 01 01 | Beckman | DU 5 |
| 21 01 11 | Beckman | Glucose-Analyzer 2 |
| 21 01 19 | Beckman | Creatinine-Analyzer 2 |
| 21 01 19 | Beckman | Urea-Analyzer 2 |
| 21 01 32 | Beckman | Clinical System 700 |
| 21 01 41 | Beckman | AS 4 / AS 8 |
| 21 01 41 | Beckman | Synchron CX3 |
| 21 01 42 | Beckman | Synchron CX 3 DELTA |
| 21 01 42 | Beckman | Synchron CX 4 |
| 21 01 42 | Beckman | Synchron CX 4 DELTA |
| 21 01 42 | Beckman | Synchron CX 5 |
| 21 01 42 | Beckman | Synchron CX 5 DELTA |
| 21 01 43 | Beckman | Synchron CX 7 |
| 21 01 43 | Beckman | Synchron CX 7 DELTA |
| 21 01 52 | Beckman | E2A |
| 21 01 53 | Beckman | ELISE |
| 21 03 01 | Beckman | PARAGON |
| 21 03 02 | Beckman | APPRAISE |
| 21 03 03 | Beckman | PARAGON CZE 2000 |
| 22 02 01 | Beckman | ICS |
| 22 02 02 | Beckman | Array 2.0 |
| 22 02 02 | Beckman | Array 360 |
| 22 02 02 | Beckman | IMAGE |
| 26 02 02 | Beckman | BIOMEK 2000 |
| 22 03 05 | Becton Dickinson | ProbeTec |
| 24 01 02 | Becton Dickinson | Sceptor |
| 24 01 02 | Becton Dickinson | Sceptorpette |
| 24 01 03 | Becton Dickinson | Bactec 460 Tb |
| 24 01 03 | Becton Dickinson | Bactec 660 |
| 24 01 03 | Becton Dickinson | Bactec 730 |
| 24 01 03 | Becton Dickinson | Bactec 860 |

| EDMA CODE | Company | Instrument-Name |
|-----------|-----------------------|-----------------------------|
| 24 01 03 | Becton Dickinson | Bactec 9000 MB |
| 24 01 03 | Becton Dickinson | Bactec 9050 |
| 24 01 03 | Becton Dickinson | Bactec 9120 |
| 24 01 03 | Becton Dickinson | Bactec 9240 |
| 23 02 01 | Becton-Dickinson | QBC I |
| 23 02 01 | Becton-Dickinson | QBC II |
| 23 02 01 | Becton-Dickinson | QBC Autoread |
| 23 03 01 | Becton-Dickinson | FACScan |
| 23 03 01 | Becton-Dickinson | FACStrak |
| 23 03 01 | Becton-Dickinson | FACSCalibur |
| 23 03 01 | Becton-Dickinson | FACSCount |
| 23 03 02 | Becton-Dickinson | FACStar ^{Plus} |
| 23 03 02 | Becton-Dickinson | FACSVantage |
| 23 03 02 | Becton-Dickinson | FACSort |
| 23 04 01 | Behnk | CL4 |
| 23 04 01 | Behnk | CL8 |
| 23 04 03 | Behnk | Thrombolyser |
| 21 05 03 | Behring | RAPIMAT |
| 22 02 01 | Behring | TurbiTimer |
| 22 02 02 | Behring | BN 100 |
| 22 02 02 | Behring | BNA |
| 22 02 02 | Behring | BN II |
| 22 03 01 | Behring | Elisa-Photometer |
| 22 03 01 | Behring | Elisa-Reader 301 |
| 22 03 01 | Behring | Elisa-Reader 311 |
| 22 03 01 | Behring | Berilux 250 |
| 22 03 01 | Behring | Microtrack Reader SE System |
| 22 03 01 | Behring | ECOM 6123 D |
| 22 03 02 | Behring | Berilux 400 |
| 22 03 02 | Behring | BEP II |
| 22 03 02 | Behring | OPUS |
| 22 03 02 | Behring | OPUS PLUS |
| 22 03 02 | Behring | ETS Plus |
| 22 03 02 | Behring | Solaris |
| 22 03 03 | Behring | OPUS Magnum |
| 22 03 04 | Behring | BEP III |
| 22 03 04 | Behring | BEP XL (Micro Trak XL) |
| 23 04 01 | Behring | Fibrintimer II |
| 23 04 01 | Behring | Fibrintimer 10 |
| 23 04 01 | Behring | Chromotimer |
| 23 04 03 | Behring | BFA |
| 23 04 03 | Behring | BCT |
| 23 04 03 | Behring | BCS |
| 21 01 12 | Bio-Rad | DIAMAT |
| 21 01 12 | Bio-Rad | VARIANT |
| 22 03 04 | Bio-Rad | Radius |
| 22 03 04 | BIO-TEK | ELx808 |
| 22 02 01 | Bio-Whittaker | Fiax |
| 22 03 01 | Biochem Immunosystems | Serazyme I |
| 22 03 01 | Biochem Immunosystems | Serazyme II |
| 22 03 02 | Biochem Immunosystems | SR 1 |
| 22 03 03 | Biochem Immunosystems | Labotec |
| 23 02 01 | Biochem Immunosystems | 130 |
| 23 02 01 | Biochem Immunosystems | 150 |

| EDMA CODE | Company | Instrument-Name |
|-----------|-----------------------|--------------------|
| 23 02 01 | Biochem Immunosystems | 170 |
| 23 02 01 | Biochem Immunosystems | 7500 |
| 23 02 01 | Biochem Immunosystems | 8000 |
| 23 02 02 | Biochem Immunosystems | 9000 |
| 23 02 02 | Biochem Immunosystems | 9100 + |
| 23 02 02 | Biochem Immunosystems | 9118 + |
| 23 02 02 | Biochem Immunosystems | 9120 + |
| 23 04 02 | Biodata | MCA 110 |
| 23 04 04 | Biodata | PAP 4 |
| 24 01 02 | Biokit | Videobact |
| 22 03 01 | BioMerieux | Axia Microreader |
| 22 03 01 | BioMerieux | Axia 2 Reader |
| 22 03 02 | BioMerieux | VIDAS |
| 22 03 02 | BioMerieux | Mini-VIDAS |
| 23 04 01 | BioMerieux | Option 2-8 |
| 23 04 03 | BioMerieux | Hemolab |
| 24 01 02 | BioMerieux | Vitek Junior |
| 24 01 02 | BioMerieux | Vitek 32 |
| 24 01 02 | BioMerieux | Vitek 60 |
| 24 01 02 | BioMerieux | Vitek 120 |
| 24 01 02 | BioMerieux | Vitek 240 |
| 24 01 02 | BioMerieux | Uniscept |
| 24 01 02 | BioMerieux | Aladin |
| 24 01 02 | BioMerieux | ATB Expression |
| 24 01 03 | BioMerieux | Vital 200 |
| 24 01 03 | BioMerieux | Vital 1200 |
| 24 01 04 | BioMerieux | Bact-T-Screen 2000 |
| 24 01 04 | BioMerieux | URIMAT |
| 21 01 01 | BioSystems | BTS 302 |
| 21 01 01 | BioSystems | BTS 305 |
| 21 01 01 | BioSystems | BTS 310 |
| 21 01 01 | Boehringer Mannheim | Photometer 4010 |
| 21 01 01 | Boehringer Mannheim | Photometer 4020 |
| 21 01 31 | Boehringer Mannheim | Reflotron |
| 21 01 31 | Boehringer Mannheim | Reflotron Sprint |
| 21 01 41 | Boehringer Mannheim | Hitachi 704 |
| 21 01 41 | Boehringer Mannheim | Hitachi 705 |
| 21 01 41 | Boehringer Mannheim | Hitachi 904 |
| 21 01 42 | Boehringer Mannheim | Hitachi 911 |
| 21 01 43 | Boehringer Mannheim | Hitachi 717 |
| 21 01 43 | Boehringer Mannheim | Hitachi 917 |
| 21 01 44 | Boehringer Mannheim | HIT 737 |
| 21 01 44 | Boehringer Mannheim | HIT 747 Series |
| 21 05 02 | Boehringer Mannheim | Urilux |
| 21 05 02 | Boehringer Mannheim | Minitron |
| 21 05 03 | Boehringer Mannheim | Miditron |
| 21 05 03 | Boehringer Mannheim | Miditron Junior |
| 21 05 03 | Boehringer Mannheim | Urotron RL 9 |
| 21 05 04 | Boehringer Mannheim | Supertron |
| 22 02 02 | Boehringer Mannheim | KeySys |
| 22 03 01 | Boehringer Mannheim | ES 11 |
| 22 03 01 | Boehringer Mannheim | ES 22 |
| 22 03 01 | Boehringer Mannheim | ES 33 |
| 22 03 02 | Boehringer Mannheim | ES 300 |

| EDMA CODE | Company | Instrument-Name |
|-----------|-----------------------------|------------------------------|
| 22 03 02 | Boehringer Mannheim | ElecSys 1010 |
| 22 03 03 | Boehringer Mannheim | ES 600 |
| 22 03 03 | Boehringer Mannheim | ES 700 |
| 22 03 03 | Boehringer Mannheim | ElecSys 2010 |
| 26 02 09 | Boehringer Mannheim | PPV |
| 23 04 02 | Boehringer Mannheim / Stago | Coasys 110 |
| 23 04 03 | Boehringer Mannheim / Stago | STA |
| 23 04 03 | Boehringer Mannheim / Stago | STA Compact |
| 22 03 02 | Byk-Sangtek | LIA-mat S 300 |
| 21 01 12 | Chiron (Ciba Corning) | Glycomat |
| 21 01 41 | Chiron (Ciba Corning) | EXPRESS |
| 21 02 01 | Chiron (Ciba Corning) | CCD 238 |
| 21 02 01 | Chiron (Ciba Corning) | CCD 248 |
| 21 02 01 | Chiron (Ciba Corning) | CCD 278 |
| 21 02 01 | Chiron (Ciba Corning) | CCD 280 |
| 21 02 01 | Chiron (Ciba Corning) | CCD 840 |
| 21 02 02 | Chiron (Ciba Corning) | CCD 348 |
| 21 02 02 | Chiron (Ciba Corning) | CCD 850 |
| 21 02 02 | Chiron (Ciba Corning) | CCD 860 |
| 21 02 04 | Chiron (Ciba Corning) | CCD 845 |
| 21 02 04 | Chiron (Ciba Corning) | CCD 855 |
| 21 02 04 | Chiron (Ciba Corning) | CCD 865 |
| 21 02 06 | Chiron (Ciba Corning) | CCD 865 |
| 21 02 07 | Chiron (Ciba Corning) | CCD 270 |
| 21 02 07 | Chiron (Ciba Corning) | CCD 815 |
| 22 03 01 | Chiron (Ciba Corning) | Magic Lite I |
| 22 03 02 | Chiron (Ciba Corning) | Magic Lite II |
| 22 03 02 | Chiron (Ciba Corning) | Magic Lite II+ |
| 22 03 02 | Chiron (Ciba Corning) | Magic Lite SQ Allergy System |
| 22 03 03 | Chiron (Ciba Corning) | ACS 180 |
| 22 03 03 | Chiron (Ciba Corning) | ACS 180 PLUS |
| 23 04 03 | Chiron (Ciba Corning) | Biotrack 512 |
| 21 01 31 | Cholestech | L.D.X |
| 22 03 03 | CIS-Bio | Cispack 4200 |
| 24 01 04 | Coral Biotechnology | Coral Wave 120 |
| 21 03 01 | COSMO | FED 3200 |
| 21 01 42 | Coulter | Optichem 500 |
| 23 02 01 | Coulter | CBC-5 |
| 23 02 01 | Coulter | M430 |
| 23 02 01 | Coulter | MD 8 |
| 23 02 01 | Coulter | ZM |
| 23 02 01 | Coulter | M530 |
| 23 02 02 | Coulter | T540 |
| 23 02 02 | Coulter | T660 |
| 23 02 02 | Coulter | MD 16 |
| 23 02 02 | Coulter | MD II |
| 23 02 02 | Coulter | S770 |
| 23 02 03 | Coulter | JS |
| 23 02 03 | Coulter | JR |
| 23 02 03 | Coulter | T890 |
| 23 02 03 | Coulter | S880 |
| 23 02 03 | Coulter | Onyx |
| 23 02 04 | Coulter | STKR |
| 23 02 04 | Coulter | STKS |

| EDMA CODE | Company | Instrument-Name |
|-----------|-------------------|-----------------------|
| 23 02 04 | Coulter | MAXM |
| 23 02 04 | Coulter | ST |
| 23 03 01 | Coulter | Epics Profile II |
| 23 03 02 | Coulter | Epics Elite |
| 22 03 02 | Dade | Stratus I |
| 22 03 02 | Dade | Stratus II |
| 24 01 02 | Dade | Touchscan |
| 24 01 02 | Dade | Autoscan 4 |
| 24 01 02 | Dade | Microscan Walkaway 40 |
| 24 01 02 | Dade | Microscan Walkaway 96 |
| 24 01 02 | Dade | Autosceptor |
| 21 01 41 | Dade (Dupont) | Dimension 380 |
| 21 01 41 | Dade (Dupont) | Dimension ES |
| 21 01 43 | Dade (Dupont) | Paramax-RX |
| 21 01 43 | Dade (Dupont) | Dimension 760 |
| 21 01 43 | Dade (Dupont) | Dimension AR |
| 21 01 43 | Dade (Dupont) | Dimension XL |
| 22 03 02 | Dade (Dupont) | ACA III |
| 22 03 02 | Dade (Dupont) | ACA V |
| 22 03 02 | Dade (Dupont) | ACA SX |
| 22 03 02 | Dade (Dupont) | ACA STAR |
| 21 02 02 | Diametrics | IRMA |
| 24 01 02 | Difco | Pasco |
| 24 01 03 | Difco | Sentinel |
| 24 01 03 | Difco | ESP |
| 24 01 04 | Difco | Questor |
| 22 03 02 | DPC | Milenia Max |
| 22 03 02 | DPC | Immulite |
| 22 03 04 | DPC / Biermann | MAX |
| 22 03 01 | Dynatech | System 5000 |
| 22 03 04 | Dynatech | System 7000 |
| 21 01 01 | Eppendorf | PCP 6121 |
| 21 01 01 | Eppendorf | ECOM 6122 |
| 21 01 01 | Eppendorf | ECOM 6124 F |
| 21 01 11 | Eppendorf | EBIO Compact |
| 21 01 29 | Eppendorf | EBIO Plus |
| 21 01 31 | Eppendorf | SPOTCHEM |
| 21 01 32 | Eppendorf | EPAC 6140 |
| 21 01 41 | Eppendorf | ACP 5040 |
| 21 01 41 | Eppendorf | EASY |
| 21 01 41 | Eppendorf | EPOS |
| 21 01 41 | Eppendorf | ELAN |
| 21 01 42 | Eppendorf | ERIS |
| 21 01 42 | Eppendorf | ETEC |
| 22 03 01 | Eppendorf | ECOM 6123 D |
| 21 03 03 | Eppendorf (JOKOO) | CTE 1000 |
| 21 03 03 | Eppendorf (JOKOO) | CTE 5000 |
| 21 01 01 | Gilford | 103 |
| 21 01 01 | Gilford | 203 |
| 22 03 04 | Hamilton | Microlab F.A.M.E. |
| 21 03 01 | Helena | NN |
| 21 03 02 | Helena | NN |
| 21 03 03 | Helena | Concept 2000 |
| 21 03 03 | Helena | REP |

| EDMA CODE | Company | Instrument-Name |
|-----------|-----------------------|------------------|
| 21 03 03 | Helena | Cardio REP |
| 21 03 03 | Helena | PRINCE-CE |
| 23 04 01 | Helena | Cascade M-4 |
| 23 04 02 | Helena | Cascade 480 |
| 22 03 01 | Hybritech | Photon II |
| 22 03 02 | Hybritech | Photon Era |
| 24 01 02 | I2R | STRSCAN |
| 21 05 02 | IMACO | URIMAC |
| 21 01 41 | Instrument. Lab. (IL) | Monarch 1000 |
| 21 01 42 | Instrument. Lab. (IL) | Monarch PLUS |
| 21 01 42 | Instrument. Lab. (IL) | Monarch 2000 |
| 21 01 43 | Instrument. Lab. (IL) | ILab 900 |
| 21 01 44 | Instrument. Lab. (IL) | ILab 1800 |
| 21 01 51 | Instrument. Lab. (IL) | IL 943 |
| 21 01 52 | Instrument. Lab. (IL) | IL 614, 644, 654 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1304 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1306 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1312 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1420 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1610 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1620 |
| 21 02 01 | Instrument. Lab. (IL) | IL BG3 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1400 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1405 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1430 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1630 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1640 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1650 |
| 21 02 02 | Instrument. Lab. (IL) | GEM PREMIER |
| 21 02 02 | Instrument. Lab. (IL) | GEM STAT |
| 21 02 02 | Instrument. Lab. (IL) | GEM 6+ |
| 21 02 02 | Instrument. Lab. (IL) | GEM PREMIER PLUS |
| 21 02 04 | Instrument. Lab. (IL) | Synthesis 25 /35 |
| 21 02 07 | Instrument. Lab. (IL) | IL 482 |
| 21 02 07 | Instrument. Lab. (IL) | IL 682 |
| 23 04 02 | Instrument. Lab. (IL) | ACL 100 |
| 23 04 02 | Instrument. Lab. (IL) | ACL 200 |
| 23 04 02 | Instrument. Lab. (IL) | ACL 300 |
| 23 04 03 | Instrument. Lab. (IL) | ACL 1000 |
| 23 04 03 | Instrument. Lab. (IL) | ACL 2000 |
| 23 04 03 | Instrument. Lab. (IL) | ACL 3000 |
| 23 04 03 | Instrument. Lab. (IL) | ACL 3000p |
| 23 04 03 | Instrument. Lab. (IL) | ACL 6000 |
| 23 04 03 | Instrument. Lab. (IL) | ACL Futura |
| 21 01 41 | Kone | Progress |
| 21 01 41 | Kone | Progress Plus |
| 21 01 41 | Kone | Specific |
| 21 01 41 | Kone | Specific Supra |
| 21 01 42 | Kone | Delta |
| 21 01 42 | Kone | Dynamic |
| 21 01 42 | Kone | Optima |
| 21 01 42 | Kone | Ultra |
| 23 02 01 | Kone | AC 900 |
| 23 02 01 | Kone | AC 920 |

| EDMA CODE | Company | Instrument-Name |
|-----------|-------------------|----------------------|
| 23 02 02 | Kone | AC 970 |
| 22 03 03 | Kone | Quartus |
| 23 04 01 | Labor | COA Data 1000-3000 |
| 23 04 01 | Labor | COA System |
| 23 04 01 | Labor | COA Screener |
| 23 04 01 | Labsystems | FP 900 |
| 23 04 01 | Labsystems | FP 910 |
| 21 01 01 | Lange (Dr. Lange) | LP 1 |
| 21 01 01 | Lange (Dr. Lange) | LP 3 |
| 21 01 01 | Lange (Dr. Lange) | LP 6A |
| 21 01 01 | Lange (Dr. Lange) | LP 400 |
| 21 01 01 | Lange (Dr. Lange) | LP 500 |
| 21 01 01 | Lange (Dr. Lange) | Miniphotometer 8 |
| 23 05 01 | Lifescreeen | QUASAR 240 |
| 23 05 01 | Lifescreeen | QUASAR 400 |
| 23 04 01 | LRE | Coatron F |
| 23 04 01 | LRE | Coatron F II |
| 23 04 02 | LRE | Coatron Jr. |
| 23 04 02 | LRE | Coatron Fx |
| 24 01 04 | Lumac | Biocounter M2300 |
| 24 01 04 | Lumac | Biocounter M3000 |
| 24 01 02 | Mast | Radius |
| 24 01 02 | Mast | Mastscan |
| 21 01 12 | Menarini | HA 8110 |
| 21 01 12 | Menarini | HA 8121 |
| 21 01 12 | Menarini | HA 8140 |
| 21 01 31 | Menarini | SPOTCHEM |
| 21 01 41 | Menarini | Classic/Artax |
| 21 01 42 | Menarini | Falcor 300 |
| 21 01 42 | Menarini | Falcor 600 |
| 21 03 03 | Menarini | HS 7 |
| 21 05 01 | Menarini | MiniAution |
| 21 05 04 | Menarini | SuperAution |
| 23 05 01 | Menarini | BOSS |
| 21 01 01 | Merck | Eclipse |
| 21 01 01 | Merck | Eclipse Plus |
| 21 01 12 | Merck | Hitachi L 9000 |
| 21 01 31 | Merck | EASY ST |
| 21 01 41 | Merck | Selectra |
| 21 01 43 | Merck | MEGA |
| 22 03 01 | Merck | Eclair |
| 22 03 01 | Merck | LM-8 |
| 22 03 04 | Merck | MIOS |
| 22 03 03 | Merck (Biotrol) | MAGIA 7000 |
| 22 03 03 | Merck (Biotrol) | MAGIA 8000 |
| 21 01 01 | Milton-Roy | Spectronic 1001+ |
| 21 01 01 | Milton-Roy | Spectronic 1101 |
| 21 01 01 | Milton-Roy | Spectronic 1201 |
| 21 01 01 | Milton-Roy | Spectronic 20 / 20 D |
| 21 01 01 | Milton-Roy | Spectronic 21 DV |
| 21 01 01 | Milton-Roy | Spectronic 21 MV |
| 21 01 01 | Milton-Roy | Spectronic 21 UVD |
| 21 01 01 | Milton-Roy | Spectronic 3000 |
| 21 01 01 | Milton-Roy | Spectronic 301 |

| EDMA CODE | Company | Instrument-Name |
|-----------|------------------------|--------------------------|
| 21 01 01 | Milton-Roy | Spectronic 401 |
| 21 01 01 | Milton-Roy | Spectronic 501 |
| 21 01 01 | Milton-Roy | Spectronic 601 |
| 22 03 01 | Murex | Micro ELISA Reader 7000 |
| 22 03 01 | Murex | Micro ELISA MRX Reader |
| 22 03 04 | Murex | DIAS System |
| 22 03 04 | Murex | MIAS System |
| 23 02 01 | Nihon Kohden | Celltak MEK-5100 |
| 23 02 02 | Nihon Kohden | Celltak-Auto |
| 21 01 42 | Nova | Nucleus |
| 21 02 01 | Nova | Stat Profile 3 |
| 21 02 02 | Nova Biomedical | Stat Profile1,2,4,5,7 |
| 21 02 02 | Nova Biomedical | Stat Profile Plus 9,10 |
| 22 02 01 | Nycomed | Card Reader |
| 23 04 01 | Nycomed | Thrombotrack |
| 21 01 41 | Olympus | AU 200 |
| 21 01 42 | Olympus | AU 510 |
| 21 01 42 | Olympus | AU 560 |
| 21 01 43 | Olympus | AU 600 |
| 21 01 44 | Olympus | AU 800 |
| 21 01 44 | Olympus | AU 1000 |
| 21 01 44 | Olympus | AU 5000 Series |
| 21 01 44 | Olympus | AU 5200 Series |
| 21 03 02 | Olympus | Fractoscan |
| 21 03 02 | Olympus | Fractoscan Junior |
| 21 03 03 | Olympus | HITE SYSTEM 310 |
| 21 03 03 | Olympus | HITE SYSTEM 320 |
| 21 03 03 | Olympus | HITE SYSTEM 620 |
| 23 05 01 | Olympus | PK 80 |
| 23 05 01 | Olympus | PK 7100 |
| 23 05 01 | Olympus | PK 7200 |
| 24 01 04 | Orbec | Ramus |
| 23 04 01 | Organon Teknika | Coag-a-Mate XM |
| 22 03 01 | Organon Teknika | Microelisa Reader 100 |
| 22 03 01 | Organon Teknika | Microelisa System |
| 22 03 02 | Organon Teknika | Auraflex |
| 22 03 03 | Organon Teknika | Tektime |
| 22 03 04 | Organon Teknika | MPP 3000 |
| 22 03 05 | Organon Teknika | NASBA QR System |
| 23 04 02 | Organon Teknika | Coag-A-Mate X2 |
| 23 04 02 | Organon Teknika | Coag-A-Mate RA 4 |
| 23 04 03 | Organon Teknika | Coag-A-Mate MDA |
| 23 04 03 | Organon Teknika | Coag-A-Mate MTX |
| 24 01 03 | Organon Teknika | BacT/Alert 120 |
| 24 01 03 | Organon Teknika | BacT/Alert 240 |
| 22 02 01 | Orion Diagnostica | Turbox |
| 22 02 01 | Orion Diagnostica | QuikRead 3 |
| 21 01 31 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) DT 60 |
| 21 01 42 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) 250 |
| 21 01 42 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) 500 |
| 21 01 43 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) 750 XRC |
| 21 01 43 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) 950 IRC |
| 22 03 02 | Ortho Diag.Syst. (J&J) | Amerlite |
| 22 03 03 | Ortho Diag.Syst. (J&J) | Amerlite PC |

| EDMA CODE | Company | Instrument-Name |
|-----------|---------------------------------|-------------------------|
| 22 03 03 | Ortho Diag.Syst. (J&J) | VITROS ECI |
| 23 03 01 | Ortho Diag.Syst. (J&J) | Cytoron Absolute |
| 26 02 02 | Ortho Diag.Syst. (J&J) | Summit Plus 2 |
| 26 02 02 | Ortho Diag.Syst. (J&J) | Summit Processor |
| 22 03 01 | Ortho Diagnostic Systems | Auto Reader 3 |
| 22 03 04 | Ortho Diagnostic Systems | Summit |
| 23 04 01 | Ortho Diagnostic Systems (MLA) | Electra 700 |
| 23 04 01 | Ortho Diagnostic Systems (MLA) | Koagulab CTS |
| 23 04 02 | Ortho Diagnostic Systems (MLA) | Electra 800 |
| 23 04 02 | Ortho Diagnostic Systems (MLA) | Electra 900 |
| 23 04 02 | Ortho Diagnostic Systems (MLA) | Electra 900 C |
| 23 04 02 | Ortho Diagnostic Systems (MLA) | Koagulab 16-605 |
| 23 04 03 | Ortho Diagnostic Systems (MLA) | Electra 1000 C |
| 23 04 03 | Ortho Diagnostic Systems (MLA) | Electra 1400 C |
| 23 04 03 | Ortho Diagnostic Systems (MLA) | Electra 1600 C |
| 23 04 04 | Ortho Diagnostic Systems / Dade | PFA-100 |
| 23 03 01 | Partec | CA-II |
| 23 03 02 | Partec | PAS-II |
| 21 01 01 | Perkin-Elmer | Lambda 11 |
| 21 01 01 | Perkin-Elmer | Lambda 12 |
| 21 01 01 | Perkin-Elmer | Lambda 14 |
| 22 03 02 | Pharmacia | UniCAP |
| 22 03 02 | Radim | BRIO |
| 21 02 01 | Radiometer | ABL 5 |
| 21 02 01 | Radiometer | ABL 30 |
| 21 02 01 | Radiometer | ABL 300 |
| 21 02 01 | Radiometer | ABL 330 |
| 21 02 01 | Radiometer | ABL 500 |
| 21 02 01 | Radiometer | ABL 510 |
| 21 02 01 | Radiometer | ABL 520 |
| 21 02 02 | Radiometer | ABL 4 |
| 21 02 02 | Radiometer | ABL 505 |
| 21 02 02 | Radiometer | ABL 620 |
| 21 02 04 | Radiometer | ABL 620 |
| 21 02 07 | Radiometer | OSM 3 |
| 24 01 02 | Radiometer | Sensititre |
| 21 01 01 | Riele | PMC 2000 |
| 21 01 01 | Riele | PM 210 |
| 21 01 01 | Riele | PM 310 |
| 21 01 31 | Roche | COBAS Ready (=SPOTCHEM) |
| 21 01 41 | Roche | COBAS BIO |
| 21 01 41 | Roche | COBAS MIRA |
| 21 01 41 | Roche | COBAS MIRA S |
| 21 01 41 | Roche | COBAS MIRA PLUS |
| 21 01 41 | Roche | COBAS FARA |
| 21 01 41 | Roche | COBAS FARA II |
| 21 01 43 | Roche | COBAS INTEGRA |
| 22 03 02 | Roche | COBAS EIA System |
| 22 03 03 | Roche | COBAS CORE |
| 22 03 03 | Roche | COBAS CORE II |
| 22 03 05 | Roche | COBAS Amplicor |
| 23 02 02 | Roche | COBAS MICROS |
| 23 02 02 | Roche | COBAS MINOS ST |
| 23 02 02 | Roche | COBAS MINOS STE |

| EDMA CODE | Company | Instrument-Name |
|-----------|----------------------------|----------------------|
| 23 02 02 | Roche | COBAS MINOS STX |
| 23 02 02 | Roche | COBAS MINOS STEX |
| 23 02 02 | Roche | COBAS MINOS VET |
| 23 02 03 | Roche | COBAS HELIOS LMG |
| 23 02 03 | Roche | COBAS HELIOS 5 Diff. |
| 23 02 04 | Roche | COBAS ARGOS LMG |
| 23 02 04 | Roche | COBAS ARGOS 5 Diff. |
| 23 02 04 | Roche | COBAS VEGA |
| 23 04 01 | Roche | Fibrometer |
| 22 03 03 | Rosys | Plato 1300 |
| 22 03 04 | Rosys | Plato 3300 |
| 22 02 02 | Sanofi Diagnostics Pasteur | QM 300 |
| 22 03 01 | Sanofi Diagnostics Pasteur | LP 400 |
| 22 03 03 | Sanofi Diagnostics Pasteur | Access |
| 22 03 04 | Sanofi Diagnostics Pasteur | AMS/LP 400 |
| 22 03 04 | Sanofi Diagnostics Pasteur | Sonata |
| 24 01 03 | Sanofi Diagnostics Pasteur | Bio Argos |
| 26 02 02 | Sanofi Diagnostics Pasteur | AMSS |
| 23 02 02 | SEAC | GENIUS |
| 21 03 01 | Sebia | NN |
| 21 03 02 | Sebia | NN |
| 21 03 03 | Sebia | HYDRASYS |
| 22 03 03 | Sorin | ETI System |
| 22 03 04 | Sorin | Omni System |
| 23 04 01 | Stago | STA 2 |
| 23 04 01 | Stago | STA 4 |
| 23 04 01 | Stago | STA 8 |
| 23 04 01 | Stago | STA 888 |
| 23 04 03 | Stratec | Stracomat |
| 23 02 01 | Sysmex | F-520 |
| 23 02 01 | Sysmex | F-820 |
| 23 02 02 | Sysmex | K-800 |
| 23 02 02 | Sysmex | K-1000 |
| 23 02 03 | Sysmex | NE-1500 |
| 23 02 03 | Sysmex | K-4500 |
| 23 02 04 | Sysmex | SF-3000 |
| 23 02 04 | Sysmex | SE-9000 |
| 23 02 04 | Sysmex | NE-8000 |
| 23 02 11 | Sysmex | R-3000 |
| 23 03 01 | Sysmex | R-2000/3000 |
| 24 01 04 | Sysmex | UF-100 |
| 23 04 03 | Sysmex / Dade | CA-1000 |
| 23 04 03 | Sysmex / Dade | CA-5000 |
| 23 04 03 | Sysmex / Dade | CA-6000 |
| 26 02 02 | Tecan | GENESIS RSP 200 |
| 22 03 02 | Tosoh | AIA 600 |
| 22 03 03 | Tosoh | AIA 1200 |
| 21 01 01 | Unicam | PU 8610 |
| 21 01 01 | Unicam | PU 8620 |
| 21 01 01 | Vitatron | IFP |
| 21 01 01 | Vitatron | ISP |
| 21 01 41 | Wako | 20R |
| 21 05 04 | Wako | NN |
| 21 01 42 | Wako | 30R |

| EDMA CODE | Company | Instrument-Name |
|------------------|--------------------|------------------------|
| 22 03 02 | Wallac / Pharmacia | Delfia |
| 22 03 03 | Wallac / Pharmacia | AutoDELFIA |
| 21 01 11 | Yellow Springs | YSI |
| 21 05 04 | Yeong Deong | NN |

EDMA CODE

Company

Instrument-Name

Alphabetical Order by Instrument Name

| | | | | |
|----|----|----|----------------------------|---------------|
| 21 | 01 | 01 | Gilford | 103 |
| 23 | 02 | 01 | Biochem Immunosystems | 130 |
| 23 | 02 | 01 | Biochem Immunosystems | 150 |
| 23 | 02 | 01 | Biochem Immunosystems | 170 |
| 21 | 01 | 01 | Gilford | 203 |
| 23 | 02 | 01 | Biochem Immunosystems | 7500 |
| 23 | 02 | 01 | Biochem Immunosystems | 8000 |
| 23 | 02 | 02 | Biochem Immunosystems | 9000 |
| 21 | 01 | 41 | Wako | 20R |
| 21 | 01 | 42 | Wako | 30R |
| 23 | 02 | 02 | Biochem Immunosystems | 9100 + |
| 23 | 02 | 02 | Biochem Immunosystems | 9118 + |
| 23 | 02 | 02 | Biochem Immunosystems | 9120 + |
| 21 | 01 | 41 | Abbott | ABA 100 / 200 |
| 21 | 02 | 01 | Radiometer | ABL 30 |
| 21 | 02 | 01 | Radiometer | ABL 300 |
| 21 | 02 | 01 | Radiometer | ABL 330 |
| 21 | 02 | 02 | Radiometer | ABL 4 |
| 21 | 02 | 01 | Radiometer | ABL 5 |
| 21 | 02 | 01 | Radiometer | ABL 500 |
| 21 | 02 | 02 | Radiometer | ABL 505 |
| 21 | 02 | 01 | Radiometer | ABL 510 |
| 21 | 02 | 01 | Radiometer | ABL 520 |
| 21 | 02 | 02 | Radiometer | ABL 620 |
| 21 | 02 | 04 | Radiometer | ABL 620 |
| 23 | 02 | 01 | Kone | AC 900 |
| 23 | 02 | 01 | Kone | AC 920 |
| 23 | 02 | 02 | Kone | AC 970 |
| 22 | 03 | 02 | Dade (Dupont) | ACA III |
| 22 | 03 | 02 | Dade (Dupont) | ACA STAR |
| 22 | 03 | 02 | Dade (Dupont) | ACA SX |
| 22 | 03 | 02 | Dade (Dupont) | ACA V |
| 22 | 03 | 03 | Sanofi Diagnostics Pasteur | Access |
| 23 | 04 | 02 | Instrument. Lab. (IL) | ACL 100 |
| 23 | 04 | 03 | Instrument. Lab. (IL) | ACL 1000 |
| 23 | 04 | 02 | Instrument. Lab. (IL) | ACL 200 |
| 23 | 04 | 03 | Instrument. Lab. (IL) | ACL 2000 |
| 23 | 04 | 02 | Instrument. Lab. (IL) | ACL 300 |
| 23 | 04 | 03 | Instrument. Lab. (IL) | ACL 3000 |
| 23 | 04 | 03 | Instrument. Lab. (IL) | ACL 3000p |
| 23 | 04 | 03 | Instrument. Lab. (IL) | ACL 6000 |
| 23 | 04 | 03 | Instrument. Lab. (IL) | ACL Futura |
| 21 | 01 | 41 | Eppendorf | ACP 5040 |
| 22 | 03 | 03 | Chiron (Ciba Corning) | ACS 180 |
| 22 | 03 | 03 | Chiron (Ciba Corning) | ACS 180 PLUS |
| 22 | 03 | 02 | Abbott | ADx |
| 22 | 03 | 03 | Tosoh | AIA 1200 |
| 22 | 03 | 02 | Tosoh | AIA 600 |
| 24 | 01 | 02 | BioMerieux | Aladin |
| 22 | 03 | 02 | Ortho Diag.Syst. (J&J) | Amerlite |
| 22 | 03 | 03 | Ortho Diag.Syst. (J&J) | Amerlite PC |
| 22 | 03 | 04 | Sanofi Diagnostics Pasteur | AMS/LP 400 |

| EDMA CODE | Company | Instrument-Name |
|-----------|----------------------------|------------------------|
| 26 02 02 | Sanofi Diagnostics Pasteur | AMSS |
| 21 03 02 | Beckman | APPRAISE |
| 22 02 02 | Beckman | Array 2.0 |
| 22 02 02 | Beckman | Array 360 |
| 21 01 41 | Beckman | AS 4 / AS 8 |
| 24 01 02 | BioMerieux | ATB Expression |
| 21 01 44 | Olympus | AU 1000 |
| 21 01 41 | Olympus | AU 200 |
| 21 01 44 | Olympus | AU 5000 Series |
| 21 01 42 | Olympus | AU 510 |
| 21 01 44 | Olympus | AU 5200 Series |
| 21 01 42 | Olympus | AU 560 |
| 21 01 43 | Olympus | AU 600 |
| 21 01 44 | Olympus | AU 800 |
| 22 03 02 | Organon Teknika | Auraflex |
| 22 03 01 | Ortho Diagnostic Systems | Auto Reader 3 |
| 22 03 03 | Wallac / Pharmacia | AutoDELFLIA |
| 24 01 02 | Dade | Autoscan 4 |
| 24 01 02 | Dade | Autosceptor |
| 21 02 07 | AVL | AVL 912 |
| 21 02 01 | AVL | AVL 945 |
| 21 02 01 | AVL | AVL 990 |
| 21 02 01 | AVL | AVL 995 |
| 22 03 01 | BioMerieux | Axia 2 Reader |
| 22 03 01 | BioMerieux | Axia Microreader |
| 21 01 43 | Bayer | AXON |
| 22 03 03 | Abbott | AxSYM |
| 24 01 04 | BioMerieux | Bact-T-Screen 2000 |
| 24 01 03 | Organon Teknika | BacT/Alert 120 |
| 24 01 03 | Organon Teknika | BacT/Alert 240 |
| 24 01 03 | Becton Dickinson | Bactec 460 Tb |
| 24 01 03 | Becton Dickinson | Bactec 660 |
| 24 01 03 | Becton Dickinson | Bactec 730 |
| 24 01 03 | Becton Dickinson | Bactec 860 |
| 24 01 03 | Becton Dickinson | Bactec 9000 MB |
| 24 01 03 | Becton Dickinson | Bactec 9050 |
| 24 01 03 | Becton Dickinson | Bactec 9120 |
| 24 01 03 | Becton Dickinson | Bactec 9240 |
| 23 04 03 | Behring | BCS |
| 23 04 03 | Behring | BCT |
| 22 03 02 | Behring | BEP II |
| 22 03 04 | Behring | BEP III |
| 22 03 04 | Behring | BEP XL (Micro Trak XL) |
| 22 03 01 | Behring | Berilux 250 |
| 22 03 02 | Behring | BeriLux 400 |
| 23 04 03 | Behring | BFA |
| 24 01 03 | Sanofi Diagnostics Pasteur | Bio Argos |
| 24 01 04 | Lumac | Biocounter M2300 |
| 24 01 04 | Lumac | Biocounter M3000 |
| 26 02 02 | Beckman | BIOMEK 2000 |
| 23 04 03 | Chiron (Ciba Corning) | Biotrack 512 |
| 22 02 02 | Behring | BN 100 |
| 22 02 02 | Behring | BN II |
| 22 02 02 | Behring | BNA |

| EDMA CODE | Company | Instrument-Name |
|-----------|-----------------------|---------------------|
| 23 05 01 | Menarini | BOSS |
| 22 03 02 | Radim | BRIO |
| 21 01 01 | BioSystems | BTS 302 |
| 21 01 01 | BioSystems | BTS 305 |
| 21 01 01 | BioSystems | BTS 310 |
| 23 04 03 | Sysmex / Dade | CA-1000 |
| 23 04 03 | Sysmex / Dade | CA-5000 |
| 23 04 03 | Sysmex / Dade | CA-6000 |
| 23 03 01 | Partec | CA-II |
| 22 02 01 | Nycomed | Card Reader |
| 21 03 03 | Helena | Cardio REP |
| 23 04 02 | Helena | Cascade 480 |
| 23 04 01 | Helena | Cascade M-4 |
| 23 02 01 | Coulter | CBC-5 |
| 21 02 01 | Chiron (Ciba Corning) | CCD 238 |
| 21 02 01 | Chiron (Ciba Corning) | CCD 248 |
| 21 02 07 | Chiron (Ciba Corning) | CCD 270 |
| 21 02 01 | Chiron (Ciba Corning) | CCD 278 |
| 21 02 01 | Chiron (Ciba Corning) | CCD 280 |
| 21 02 02 | Chiron (Ciba Corning) | CCD 348 |
| 21 02 07 | Chiron (Ciba Corning) | CCD 815 |
| 21 02 01 | Chiron (Ciba Corning) | CCD 840 |
| 21 02 04 | Chiron (Ciba Corning) | CCD 845 |
| 21 02 02 | Chiron (Ciba Corning) | CCD 850 |
| 21 02 04 | Chiron (Ciba Corning) | CCD 855 |
| 21 02 02 | Chiron (Ciba Corning) | CCD 860 |
| 21 02 04 | Chiron (Ciba Corning) | CCD 865 |
| 21 02 06 | Chiron (Ciba Corning) | CCD 865 |
| 23 02 02 | Abbott | CELL-DYN 1300 |
| 23 02 02 | Abbott | CELL-DYN 1400 |
| 23 02 02 | Abbott | CELL-DYN 1600 |
| 23 02 02 | Abbott | CELL-DYN 1700 |
| 23 02 03 | Abbott | CELL-DYN 2000 |
| 23 02 01 | Abbott | CELL-DYN 300 |
| 23 02 04 | Abbott | CELL-DYN 3000 |
| 23 02 04 | Abbott | CELL-DYN 3500 |
| 23 02 01 | Abbott | CELL-DYN 400 |
| 23 02 04 | Abbott | CELL-DYN 4000 |
| 23 02 01 | Abbott | CELL-DYN 500 |
| 23 02 01 | Abbott | CELL-DYN 610 |
| 23 02 01 | Abbott | CELL-DYN 700 |
| 23 02 01 | Abbott | CELL-DYN 800 |
| 23 02 01 | Abbott | CELL-DYN 900 |
| 23 02 01 | Nihon Kohden | Celltak MEK-5100 |
| 23 02 02 | Nihon Kohden | Celltak-Auto |
| 21 01 44 | Bayer | CHEM 1 |
| 23 04 01 | Behring | Chromotimer |
| 22 03 03 | CIS-Bio | Cispack 4200 |
| 23 04 01 | Behnk | CL4 |
| 23 04 01 | Behnk | CL8 |
| 21 01 41 | Menarini | Classic/Artax |
| 21 01 32 | Beckman | Clinical System 700 |
| 21 05 02 | Bayer | Clinitek 100 |
| 21 05 03 | Bayer | Clinitek 200 |

| EDMA CODE | Company | Instrument-Name |
|-----------|-----------------------------|-------------------------|
| 21 05 03 | Bayer | Clinitek 200 + |
| 21 05 02 | Bayer | Clinitek 50 |
| 21 05 04 | Bayer | Clinitek Atlas |
| 23 04 01 | Labor | COA Data 1000-3000 |
| 23 04 01 | Labor | COA Screener |
| 23 04 01 | Labor | COA System |
| 23 04 03 | Organon Teknika | Coag-A-Mate MDA |
| 23 04 03 | Organon Teknika | Coag-A-Mate MTX |
| 23 04 02 | Organon Teknika | Coag-A-Mate RA 4 |
| 23 04 02 | Organon Teknika | Coag-A-Mate X2 |
| 23 04 01 | Organon Teknika | Coag-a-Mate XM |
| 23 04 02 | Boehringer Mannheim / Stago | Coasys 110 |
| 23 04 01 | LRE | Coatron F |
| 23 04 01 | LRE | Coatron F II |
| 23 04 02 | LRE | Coatron Fx |
| 23 04 02 | LRE | Coatron Jr. |
| 22 03 05 | Roche | COBAS Amplicor |
| 23 02 04 | Roche | COBAS ARGOS 5 Diff. |
| 23 02 04 | Roche | COBAS ARGOS LMG |
| 21 01 41 | Roche | COBAS BIO |
| 22 03 03 | Roche | COBAS CORE |
| 22 03 03 | Roche | COBAS CORE II |
| 22 03 02 | Roche | COBAS EIA System |
| 21 01 41 | Roche | COBAS FARA |
| 21 01 41 | Roche | COBAS FARA II |
| 23 02 03 | Roche | COBAS HELIOS 5 Diff. |
| 23 02 03 | Roche | COBAS HELIOS LMG |
| 21 01 43 | Roche | COBAS INTEGRA |
| 23 02 02 | Roche | COBAS MICROS |
| 23 02 02 | Roche | COBAS MINOS ST |
| 23 02 02 | Roche | COBAS MINOS STE |
| 23 02 02 | Roche | COBAS MINOS STEX |
| 23 02 02 | Roche | COBAS MINOS STX |
| 23 02 02 | Roche | COBAS MINOS VET |
| 21 01 41 | Roche | COBAS MIRA |
| 21 01 41 | Roche | COBAS MIRA PLUS |
| 21 01 41 | Roche | COBAS MIRA S |
| 21 01 31 | Roche | COBAS Ready (=SPOTCHEM) |
| 23 02 04 | Roche | COBAS VEGA |
| 22 03 04 | Abbott | Commander / FPC |
| 21 02 01 | AVL | Compact 1 |
| 21 02 01 | AVL | Compact 2 |
| 21 03 03 | Helena | Concept 2000 |
| 24 01 04 | Coral Biotechnology | Coral Wave 120 |
| 21 01 19 | Beckman | Creatinine-Analyzer 2 |
| 21 03 03 | Eppendorf (JOKOO) | CTE 1000 |
| 21 03 03 | Eppendorf (JOKOO) | CTE 5000 |
| 23 03 01 | Ortho Diag.Syst. (J&J) | Cytoron Absolute |
| 21 01 43 | Bayer | DAX 24 |
| 21 01 43 | Bayer | DAX 48 |
| 21 01 44 | Bayer | DAX 72 |
| 21 01 44 | Bayer | DAX 96 |
| 21 01 12 | Bayer | DCA 2000 |
| 22 03 02 | Wallac / Pharmacia | Delfia |

| EDMA CODE | Company | Instrument-Name |
|-----------|--------------------------------|------------------|
| 21 01 42 | Kone | Delta |
| 21 01 12 | Bio-Rad | DIAMAT |
| 22 03 04 | Murex | DIAS System |
| 21 01 41 | Dade (Dupont) | Dimension 380 |
| 21 01 43 | Dade (Dupont) | Dimension 760 |
| 21 01 43 | Dade (Dupont) | Dimension AR |
| 21 01 41 | Dade (Dupont) | Dimension ES |
| 21 01 43 | Dade (Dupont) | Dimension XL |
| 22 02 02 | Bayer | DPA-1 |
| 21 01 01 | Beckman | DU 5 |
| 21 01 42 | Kone | Dynamic |
| 21 01 52 | Beckman | E2A |
| 21 01 41 | Eppendorf | EASY |
| 21 01 31 | Merck | EASY ST |
| 21 01 11 | Eppendorf | EBIO Compact |
| 21 01 29 | Eppendorf | EBIO Plus |
| 22 03 01 | Merck | Eclair |
| 21 01 01 | Merck | Eclipse |
| 21 01 01 | Merck | Eclipse Plus |
| 21 01 01 | Eppendorf | ECOM 6122 |
| 22 03 01 | Behring | ECOM 6123 D |
| 22 03 01 | Eppendorf | ECOM 6123 D |
| 21 01 01 | Eppendorf | ECOM 6124 F |
| 21 01 41 | Eppendorf | ELAN |
| 22 03 02 | Boehringer Mannheim | ElecSys 1010 |
| 22 03 03 | Boehringer Mannheim | ElecSys 2010 |
| 23 04 03 | Ortho Diagnostic Systems (MLA) | Electra 1000 C |
| 23 04 03 | Ortho Diagnostic Systems (MLA) | Electra 1400 C |
| 23 04 03 | Ortho Diagnostic Systems (MLA) | Electra 1600 C |
| 23 04 01 | Ortho Diagnostic Systems (MLA) | Electra 700 |
| 23 04 02 | Ortho Diagnostic Systems (MLA) | Electra 800 |
| 23 04 02 | Ortho Diagnostic Systems (MLA) | Electra 900 |
| 23 04 02 | Ortho Diagnostic Systems (MLA) | Electra 900 C |
| 22 03 01 | Behring | Elisa-Photometer |
| 22 03 01 | Behring | Elisa-Reader 301 |
| 22 03 01 | Behring | Elisa-Reader 311 |
| 21 01 53 | Beckman | ELISE |
| 22 03 04 | BIO-TEK | ELx808 |
| 21 01 32 | Eppendorf | EPAC 6140 |
| 23 03 02 | Coulter | Epics Elite |
| 23 03 01 | Coulter | Epics Profile II |
| 21 01 41 | Eppendorf | EPOS |
| 21 01 42 | Abbott | EPx |
| 21 01 42 | Eppendorf | ERIS |
| 22 03 01 | Boehringer Mannheim | ES 11 |
| 22 03 01 | Boehringer Mannheim | ES 22 |
| 22 03 02 | Boehringer Mannheim | ES 300 |
| 22 03 01 | Boehringer Mannheim | ES 33 |
| 22 03 03 | Boehringer Mannheim | ES 600 |
| 22 03 03 | Boehringer Mannheim | ES 700 |
| 24 01 03 | Difco | ESP |
| 21 01 42 | Eppendorf | ETEC |
| 22 03 03 | Sorin | ETI System |
| 22 03 02 | Behring | ETS Plus |

| EDMA CODE | Company | Instrument-Name |
|-----------|-----------------------|-------------------------|
| 21 01 41 | Chiron (Ciba Corning) | EXPRESS |
| 23 02 01 | Sysmex | F-520 |
| 23 02 01 | Sysmex | F-820 |
| 23 03 01 | Becton-Dickinson | FACSCalibur |
| 23 03 01 | Becton-Dickinson | FACScan |
| 23 03 01 | Becton-Dickinson | FACSCount |
| 23 03 02 | Becton-Dickinson | FACSort |
| 23 03 02 | Becton-Dickinson | FACStar ^{Plus} |
| 23 03 01 | Becton-Dickinson | FACStrak |
| 23 03 02 | Becton-Dickinson | FACSVantage |
| 21 01 42 | Menarini | Falcor 300 |
| 21 01 42 | Menarini | Falcor 600 |
| 21 03 01 | COSMO | FED 3200 |
| 22 02 01 | Bio-Whittaker | Fiax |
| 23 04 01 | Behring | Fibrintimer 10 |
| 23 04 01 | Behring | Fibrintimer II |
| 23 04 01 | Roche | Fibrometer |
| 23 04 01 | Labsystems | FP 900 |
| 23 04 01 | Labsystems | FP 910 |
| 21 03 02 | Olympus | Fractoscan |
| 21 03 02 | Olympus | Fractoscan Junior |
| 21 02 02 | Instrument. Lab. (IL) | GEM 6+ |
| 21 02 02 | Instrument. Lab. (IL) | GEM PREMIER |
| 21 02 02 | Instrument. Lab. (IL) | GEM PREMIER PLUS |
| 21 02 02 | Instrument. Lab. (IL) | GEM STAT |
| 26 02 02 | Tecan | GENESIS RSP 200 |
| 23 02 02 | SEAC | GENIUS |
| 21 01 11 | Beckman | Glucose-Analyzer 2 |
| 21 01 12 | Chiron (Ciba Corning) | Glycomat |
| 23 02 04 | Bayer | H 1 E |
| 23 02 04 | Bayer | H 2 |
| 23 02 04 | Bayer | H 3 RTC |
| 23 02 04 | Bayer | H 3 RTX |
| 23 02 03 | Bayer | H1 |
| 23 02 02 | Bayer | H1JR |
| 21 01 12 | Menarini | HA 8110 |
| 21 01 12 | Menarini | HA 8121 |
| 21 01 12 | Menarini | HA 8140 |
| 23 04 03 | BioMerieux | Hemolab |
| 21 01 44 | Boehringer Mannheim | HIT 737 |
| 21 01 44 | Boehringer Mannheim | HIT 747 Series |
| 21 01 12 | Merck | Hitachi L 9000 |
| 21 01 41 | Boehringer Mannheim | Hitachi 704 |
| 21 01 41 | Boehringer Mannheim | Hitachi 705 |
| 21 01 43 | Boehringer Mannheim | Hitachi 717 |
| 21 01 41 | Boehringer Mannheim | Hitachi 904 |
| 21 01 42 | Boehringer Mannheim | Hitachi 911 |
| 21 01 43 | Boehringer Mannheim | Hitachi 917 |
| 21 03 03 | Olympus | HITE SYSTEM 310 |
| 21 03 03 | Olympus | HITE SYSTEM 320 |
| 21 03 03 | Olympus | HITE SYSTEM 620 |
| 21 03 03 | Menarini | HS 7 |
| 21 03 03 | Sebia | HYDRASYS |
| 22 02 01 | Beckman | ICS |

| EDMA CODE | Company | Instrument-Name |
|-----------|--------------------------------|------------------|
| 21 01 01 | Vitatron | IFP |
| 21 02 01 | Instrument. Lab. (IL) | IL 1304 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1306 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1312 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1400 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1405 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1420 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1430 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1610 |
| 21 02 01 | Instrument. Lab. (IL) | IL 1620 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1630 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1640 |
| 21 02 02 | Instrument. Lab. (IL) | IL 1650 |
| 21 02 07 | Instrument. Lab. (IL) | IL 482 |
| 21 01 52 | Instrument. Lab. (IL) | IL 614, 644, 654 |
| 21 02 07 | Instrument. Lab. (IL) | IL 682 |
| 21 01 51 | Instrument. Lab. (IL) | IL 943 |
| 21 02 01 | Instrument. Lab. (IL) | IL BG3 |
| 21 01 44 | Instrument. Lab. (IL) | ILab 1800 |
| 21 01 43 | Instrument. Lab. (IL) | ILab 900 |
| 22 02 02 | Beckman | IMMAGE |
| 22 03 02 | DPC | Immulite |
| 22 03 03 | Bayer | Immuno-I |
| 22 03 02 | Abbott | IMx / IMx Select |
| 21 02 02 | Diametrics | IRMA |
| 21 01 01 | Vitatron | ISP |
| 23 02 03 | Coulter | JR |
| 23 02 03 | Coulter | JS |
| 23 02 02 | Sysmex | K-1000 |
| 23 02 03 | Sysmex | K-4500 |
| 23 02 02 | Sysmex | K-800 |
| 23 04 01 | Amelung | KC 10 |
| 23 04 01 | Amelung | KC 10A |
| 23 04 01 | Amelung | KC 4 |
| 23 04 03 | Amelung | KC 40 |
| 22 02 02 | Boehringer Mannheim | KeySys |
| 23 04 02 | Ortho Diagnostic Systems (MLA) | Koagulab 16-605 |
| 23 04 01 | Ortho Diagnostic Systems (MLA) | Koagulab CTS |
| 21 01 31 | Cholestech | L.D.X |
| 22 03 03 | Biochem Immunosystems | Labotec |
| 21 01 01 | Perkin-Elmer | Lambda 11 |
| 21 01 01 | Perkin-Elmer | Lambda 12 |
| 21 01 01 | Perkin-Elmer | Lambda 14 |
| 22 03 05 | Abbott | LCx |
| 22 03 02 | Byk-Sangtek | LIA-mat S 300 |
| 22 03 01 | Merck | LM-8 |
| 21 01 01 | Lange (Dr. Lange) | LP 1 |
| 21 01 01 | Lange (Dr. Lange) | LP 3 |
| 21 01 01 | Lange (Dr. Lange) | LP 400 |
| 22 03 01 | Sanofi Diagnostics Pasteur | LP 400 |
| 21 01 01 | Lange (Dr. Lange) | LP 500 |
| 21 01 01 | Lange (Dr. Lange) | LP 6A |
| 23 02 01 | Coulter | M430 |
| 23 02 01 | Coulter | M530 |

| EDMA CODE | Company | Instrument-Name |
|-----------|-----------------------|------------------------------|
| 22 03 03 | Merck (Biotrol) | MAGIA 7000 |
| 22 03 03 | Merck (Biotrol) | MAGIA 8000 |
| 22 03 01 | Chiron (Ciba Corning) | Magic Lite I |
| 22 03 02 | Chiron (Ciba Corning) | Magic Lite II |
| 22 03 02 | Chiron (Ciba Corning) | Magic Lite II+ |
| 22 03 02 | Chiron (Ciba Corning) | Magic Lite SQ Allergy System |
| 24 01 02 | Mast | Mastascan |
| 22 03 01 | Abbott | Matrix |
| 22 03 04 | DPC / Biermann | MAX |
| 23 02 04 | Coulter | MAXM |
| 23 04 02 | Biodata | MCA 110 |
| 23 02 02 | Coulter | MD 16 |
| 23 02 01 | Coulter | MD 8 |
| 23 02 02 | Coulter | MD II |
| 21 01 43 | Merck | MEGA |
| 22 03 04 | Murex | MIAS System |
| 22 03 01 | Murex | Micro ELISA MRX Reader |
| 22 03 01 | Murex | Micro ELISA Reader 7000 |
| 22 03 01 | Organon Teknika | Microelisa Reader 100 |
| 22 03 01 | Organon Teknika | Microelisa System |
| 22 03 04 | Hamilton | Microlab F.A.M.E. |
| 24 01 02 | Dade | Microscan Walkaway 40 |
| 24 01 02 | Dade | Microscan Walkaway 96 |
| 22 03 01 | Behring | Microtrack Reader SE System |
| 21 05 03 | Boehringer Mannheim | Miditron |
| 21 05 03 | Boehringer Mannheim | Miditron Junior |
| 22 03 02 | DPC | Milenia Max |
| 22 03 02 | BioMerieux | Mini-VIDAS |
| 21 05 01 | Menarini | MiniAution |
| 21 01 01 | Lange (Dr. Lange) | Miniphotometer 8 |
| 21 05 02 | Boehringer Mannheim | Minitron |
| 22 03 04 | Merck | MIOS |
| 21 01 01 | Bayer | ML 1 |
| 21 01 01 | Bayer | ML2 |
| 21 01 01 | Bayer | ML3 |
| 21 01 01 | Beckman | Model 42 |
| 21 01 41 | Instrument. Lab. (IL) | Monarch 1000 |
| 21 01 42 | Instrument. Lab. (IL) | Monarch 2000 |
| 21 01 42 | Instrument. Lab. (IL) | Monarch PLUS |
| 22 03 04 | Organon Teknika | MPP 3000 |
| 22 03 05 | Organon Teknika | NASBA QR System |
| 23 02 03 | Sysmex | NE-1500 |
| 23 02 04 | Sysmex | NE-8000 |
| 21 03 01 | Helena | NN |
| 21 03 02 | Helena | NN |
| 21 03 01 | Sebia | NN |
| 21 03 02 | Sebia | NN |
| 21 05 04 | Wako | NN |
| 21 05 04 | Yeong Deong | NN |
| 21 01 42 | Nova | Nucleus |
| 21 02 04 | AVL | OMNI |
| 22 03 04 | Sorin | Omni System |
| 23 02 03 | Coulter | Onyx |
| 21 01 42 | Bayer | OPERA |

| EDMA CODE | Company | Instrument-Name |
|-----------|---------------------------------|-------------------|
| 21 02 01 | AVL | OPTI 1 |
| 21 01 42 | Coulter | Optichem 500 |
| 21 01 42 | Kone | Optima |
| 23 04 01 | BioMerieux | Option 2-8 |
| 22 03 02 | Behring | OPUS |
| 22 03 03 | Behring | OPUS Magnum |
| 22 03 02 | Behring | OPUS PLUS |
| 21 02 07 | Radiometer | OSM 3 |
| 23 04 04 | Biodata | PAP 4 |
| 21 03 01 | Beckman | PARAGON |
| 21 03 03 | Beckman | PARAGON CZE 2000 |
| 21 01 43 | Dade (Dupont) | Paramax-RX |
| 23 03 02 | Partec | PAS-II |
| 24 01 02 | Difco | Pasco |
| 21 01 01 | Eppendorf | PCP 6121 |
| 21 01 43 | American Monitor | Perspective/Excel |
| 23 04 04 | Ortho Diagnostic Systems / Dade | PFA-100 |
| 21 01 01 | Boehringer Mannheim | Photometer 4010 |
| 21 01 01 | Boehringer Mannheim | Photometer 4020 |
| 22 03 02 | Hybritech | Photon Era |
| 22 03 01 | Hybritech | Photon II |
| 23 05 01 | Olympus | PK 7100 |
| 23 05 01 | Olympus | PK 7200 |
| 23 05 01 | Olympus | PK 80 |
| 22 03 03 | Rosys | Plato 1300 |
| 22 03 04 | Rosys | Plato 3300 |
| 21 01 01 | Riele | PM 210 |
| 21 01 01 | Riele | PM 310 |
| 21 01 01 | Riele | PMC 2000 |
| 26 02 02 | Abbott | PPC |
| 26 02 09 | Boehringer Mannheim | PPV |
| 21 03 03 | Helena | PRINCE-CE |
| 22 03 04 | Abbott | PRISM |
| 22 03 05 | Becton Dickinson | ProbeTec |
| 21 01 41 | Kone | Progress |
| 21 01 41 | Kone | Progress Plus |
| 21 01 01 | Unicam | PU 8610 |
| 21 01 01 | Unicam | PU 8620 |
| 23 02 01 | Becton-Dickinson | QBC Autoread |
| 23 02 01 | Becton-Dickinson | QBC I |
| 23 02 01 | Becton-Dickinson | QBC II |
| 22 02 02 | Sanofi Diagnostics Pasteur | QM 300 |
| 22 03 01 | Abbott | Quantum |
| 22 03 01 | Abbott | Quantum II |
| 22 03 03 | Kone | Quartus |
| 23 05 01 | Lifescreeen | QUASAR 240 |
| 23 05 01 | Lifescreeen | QUASAR 400 |
| 24 01 04 | Difco | Questor |
| 22 02 01 | Orion Diagnostica | QuikRead 3 |
| 23 03 01 | Sysmex | R-2000/3000 |
| 23 02 11 | Sysmex | R-3000 |
| 21 01 41 | Bayer | RA 1000 |
| 21 01 41 | Bayer | RA 50 |
| 21 01 41 | Bayer | RA 500 |

| EDMA CODE | Company | Instrument-Name |
|-----------|-----------------------------|------------------------|
| 21 01 41 | Bayer | RA XT |
| 21 01 42 | Bayer | RA2000 |
| 22 03 04 | Bio-Rad | Radius |
| 24 01 02 | Mast | Radius |
| 24 01 04 | Orbec | Ramus |
| 21 05 03 | Behring | RAPIMAT |
| 21 01 31 | Boehringer Mannheim | Reflotron |
| 21 01 31 | Boehringer Mannheim | Reflotron Sprint |
| 21 03 03 | Helena | REP |
| 23 02 02 | Coulter | S770 |
| 23 02 03 | Coulter | S880 |
| 24 01 02 | Becton Dickinson | Sceptor |
| 24 01 02 | Becton Dickinson | Sceptorpette |
| 23 02 04 | Sysmex | SE-9000 |
| 21 01 41 | Merck | Selectra |
| 24 01 02 | Radiometer | Sensititre |
| 24 01 03 | Difco | Sentinel |
| 21 01 31 | Bayer | Seralyzer |
| 22 03 01 | Biochem Immunosystems | Serazyme I |
| 22 03 01 | Biochem Immunosystems | Serazyme II |
| 23 02 04 | Sysmex | SF-3000 |
| 22 03 02 | Behring | Solaris |
| 22 03 04 | Sanofi Diagnostics Pasteur | Sonata |
| 21 01 41 | Kone | Specific |
| 21 01 41 | Kone | Specific Supra |
| 21 01 01 | Milton-Roy | Spectronic 1001+ |
| 21 01 01 | Milton-Roy | Spectronic 1101 |
| 21 01 01 | Milton-Roy | Spectronic 1201 |
| 21 01 01 | Milton-Roy | Spectronic 20 / 20 D |
| 21 01 01 | Milton-Roy | Spectronic 21 DV |
| 21 01 01 | Milton-Roy | Spectronic 21 MV |
| 21 01 01 | Milton-Roy | Spectronic 21 UVD |
| 21 01 01 | Milton-Roy | Spectronic 3000 |
| 21 01 01 | Milton-Roy | Spectronic 301 |
| 21 01 01 | Milton-Roy | Spectronic 401 |
| 21 01 01 | Milton-Roy | Spectronic 501 |
| 21 01 01 | Milton-Roy | Spectronic 601 |
| 21 01 41 | Abbott | Spectrum |
| 21 01 31 | Eppendorf | SPOTCHEM |
| 21 01 31 | Menarini | SPOTCHEM |
| 22 03 02 | Biochem Immunosystems | SR 1 |
| 23 02 04 | Coulter | ST |
| 23 04 03 | Boehringer Mannheim / Stago | STA |
| 23 04 01 | Stago | STA 2 |
| 23 04 01 | Stago | STA 4 |
| 23 04 01 | Stago | STA 8 |
| 23 04 01 | Stago | STA 888 |
| 23 04 03 | Boehringer Mannheim / Stago | STA Compact |
| 21 02 01 | Nova | Stat Profile 3 |
| 21 02 02 | Nova Biomedical | Stat Profile Plus 9,10 |
| 21 02 02 | Nova Biomedical | Stat Profile1,2,4,5,7 |
| 23 02 04 | Coulter | STKR |
| 23 02 04 | Coulter | STKS |
| 23 04 03 | Stratec | Stracomat |

| EDMA CODE | Company | Instrument-Name |
|-----------|--------------------------|--------------------------|
| 22 03 02 | Dade | Stratus I |
| 22 03 02 | Dade | Stratus II |
| 24 01 02 | I2R | STRSCAN |
| 22 03 04 | Ortho Diagnostic Systems | Summit |
| 26 02 02 | Ortho Diag.Syst. (J&J) | Summit Plus 2 |
| 26 02 02 | Ortho Diag.Syst. (J&J) | Summit Processor |
| 21 05 04 | Menarini | SuperAution |
| 21 05 04 | Boehringer Mannheim | Supertron |
| 21 01 42 | Beckman | Synchron CX 3 DELTA |
| 21 01 42 | Beckman | Synchron CX 4 |
| 21 01 42 | Beckman | Synchron CX 4 DELTA |
| 21 01 42 | Beckman | Synchron CX 5 |
| 21 01 42 | Beckman | Synchron CX 5 DELTA |
| 21 01 43 | Beckman | Synchron CX 7 |
| 21 01 43 | Beckman | Synchron CX 7 DELTA |
| 21 01 41 | Beckman | Synchron CX3 |
| 21 02 04 | Instrument. Lab. (IL) | Synthesis 25 /35 |
| 22 03 01 | Dynatech | System 5000 |
| 22 03 04 | Dynatech | System 7000 |
| 23 02 02 | Coulter | T540 |
| 23 02 02 | Coulter | T660 |
| 23 02 03 | Coulter | T890 |
| 22 03 02 | Abbott | TDx / TDxFLx |
| 22 03 03 | Organon Teknika | Tektime |
| 23 04 03 | Behnk | Thrombolysar |
| 23 04 01 | Nycomed | Thrombotrack |
| 24 01 02 | Dade | Touchscan |
| 22 02 01 | Behring | TurbiTimer |
| 22 02 01 | Orion Diagnostica | Turbox |
| 24 01 04 | Sysmex | UF-100 |
| 21 01 42 | Kone | Ultra |
| 22 03 02 | Pharmacia | UniCAP |
| 24 01 02 | BioMerieux | Uniscept |
| 21 01 19 | Beckman | Urea-Analyzer 2 |
| 21 05 02 | Boehringer Mannheim | Urilux |
| 21 05 02 | IMACO | URIMAC |
| 24 01 04 | BioMerieux | URIMAT |
| 21 05 03 | Boehringer Mannheim | Urotron RL 9 |
| 21 01 12 | Bio-Rad | VARIANT |
| 22 03 02 | BioMerieux | VIDAS |
| 24 01 02 | Biokit | Videobact |
| 21 01 31 | Abbott | Vision |
| 24 01 03 | BioMerieux | Vital 1200 |
| 24 01 03 | BioMerieux | Vital 200 |
| 24 01 02 | BioMerieux | Vitek 120 |
| 24 01 02 | BioMerieux | Vitek 240 |
| 24 01 02 | BioMerieux | Vitek 32 |
| 24 01 02 | BioMerieux | Vitek 60 |
| 24 01 02 | BioMerieux | Vitek Junior |
| 22 03 03 | Ortho Diag.Syst. (J&J) | VITROS ECI |
| 21 01 42 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) 250 |
| 21 01 42 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) 500 |
| 21 01 43 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) 750 XRC |
| 21 01 43 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) 950 IRC |

| EDMA CODE | Company | Instrument-Name |
|------------------|------------------------|------------------------|
| 21 01 31 | Ortho Diag.Syst. (J&J) | VITROS(Ektachem) DT 60 |
| 21 01 41 | Abbott | VP |
| 21 01 11 | Yellow Springs | YSI |
| 23 02 01 | Coulter | ZM |